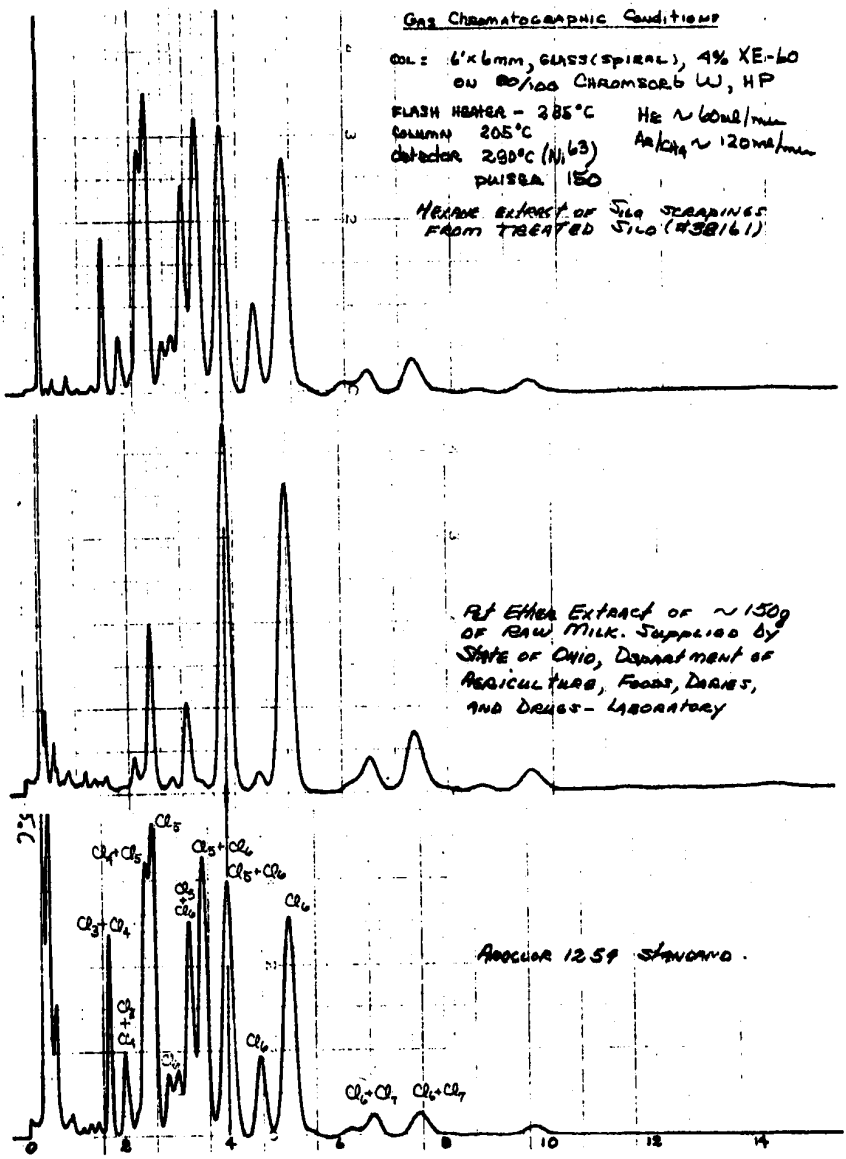
Gas Chromatographic Conditions
COL: 6'x6mm, GLASS (SPIRAL), 4% XE-60 on 80/100 CHROMSORB W, HP
FLASH HEATER - 285°C
COLUMN 205°C
detector 280°C (Ni 63)
PULSER 150
He ~60ml/min
Ar/CH4 ~120ml/min
HEXANE EXTRACT OF SILO SCRAPINGS FROM TREATED SILO (#38161)
Pet Ether Extract of ~150g of RAW MILK. Supplied by State of Ohio, Department of Agriculture, Foods, Drugs, and Drugs - Laboratory
AROCLOR 1259 STANDARD.
Cl5
Cl4+Cl5
Cl5+Cl6
Cl3+Cl4
Cl5+Cl6
Cl6
Cl2+Cl3
Cl6
Cl6+Cl7
Cl6+Cl7
0
2
4
6
8
10
12
14

MONS 096437

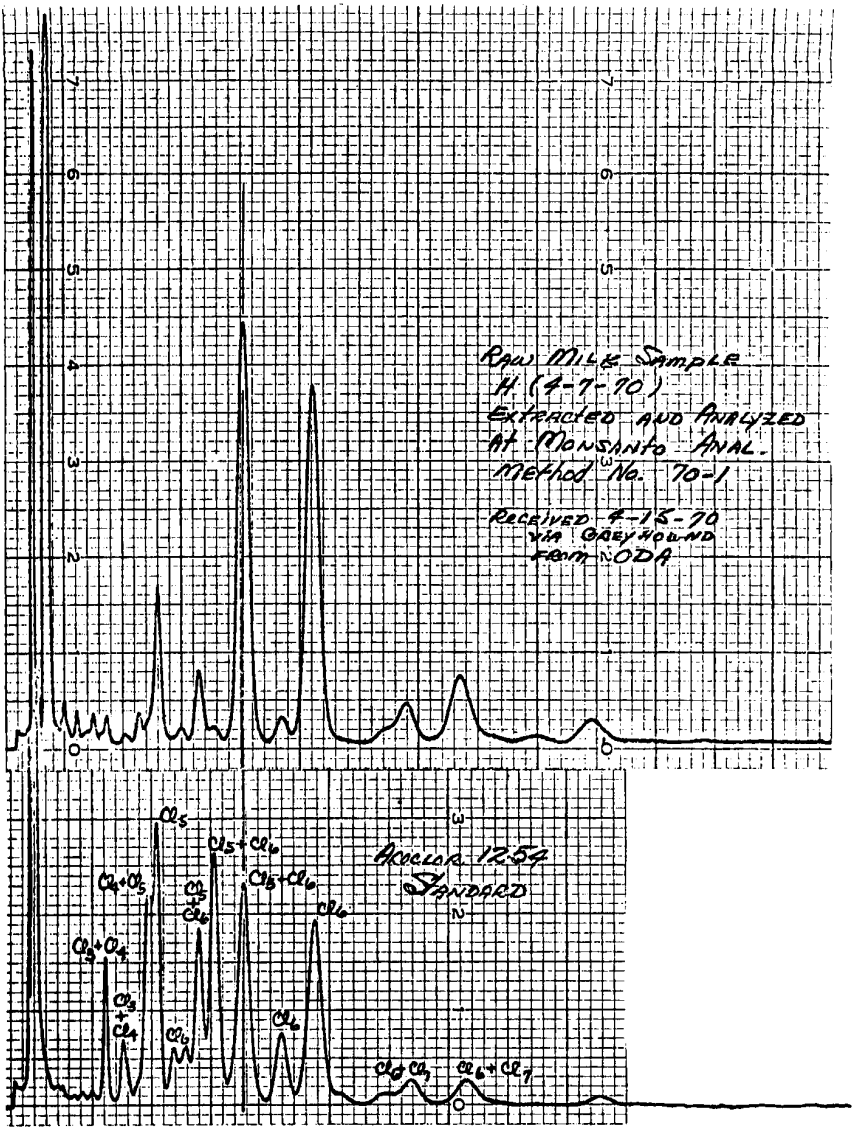
RAW MILK SAMPLE
H (4-7-70)
EXTRACTED AND ANALYZED
AT MONSANTO ANAL.
METHOD NO. 70-1
RECEIVED 4-15-70
VIA GREYHOUND
FROM ODA
AROCLOR 1254
STANDARD
Cl5
Cl5+Cl6
Cl4+Cl5
Cl5+Cl6
Cl6
Cl3+Cl4
Cl3+Cl4
Cl6
Cl6
Cl6
Cl6 Cl7
Cl6+Cl7