



LABORATOIRE D'HYGIENE ET DE
CONTROLE DES FIBRES MINÉRALES

10, rue de la Pépinière, 75008 PARIS
Tél. (1) 45 22 12 34 - Fax 42 94 98 86

Paris, September 17th 1990

Mrs Janis WOODSON REYNOLDS

CERTAINTEED CORPORATION
750 E. Swedesford Road
Valley Forge05
PA, 19482
U.S.A.

RECEIVED SEP 21 1990

Ref. : A.I.A. Fibre Counting Trial 1990

Dear Mrs WOODSON,

I acknowledge receipt of the counting results of 3
counters from your laboratory.

You will find enclosed a provisional report giving
the individual positions of these counters according to the 3
groups.

The final report should be circulated at the end of
the year, in which counting results of each participant will
be taken into account.

Yours sincerely.

Alain Baujon
Director

PLAINTIFF'S EXHIBIT

CT-671

CTD026253

A.I.A. - FIBRE COUNTING TRIAL - 1990

PROVISIONAL POSITION DATA SHEET


Name : Mr Scott HOWARD
Company : CERTAINTEED

Your countings and corresponding normalised results are reported below.

Slide Ref. : D	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15
Results F/mm ²	126	745	375	142	339	93	120	228	277	673	78	290	379	250	127
Norm. Results	1.34	2.27	2.39	0.61	2.25	0.52	1.51	2.45	0.96	5.77	0.17	4.80	2.45	0.86	0.70

Normalised Mean : 1.94
Coefficient of Variation : 81.5

Your individual position is plotted on the following diagram:

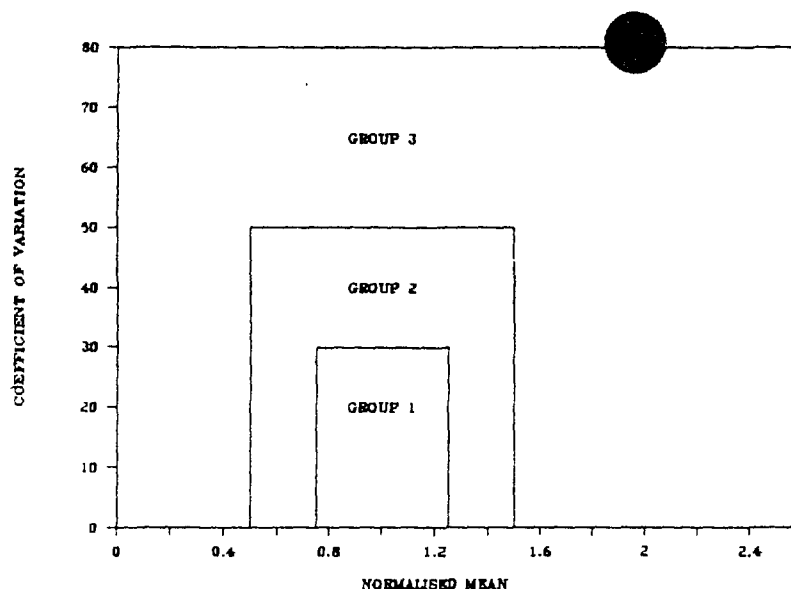

Group 1 : Counters with normalised mean in the range
0,75 - 1,25 and coefficient of variation below 30 %

Group 2 : Counters with normalised mean in the range
0,5 - 1,5 and coefficient of variation below 50 %

Group 3 : Counters with normalised mean outside the range
0,5 - 1,5 or coefficient of variation above 50 %

A.I.A. - FIBRE COUNTING TRIAL - 1990

PROVISIONAL POSITION DATA SHEET


Name : Mrs Janis WOODSON REYNOLDS
Company : CERTAINTEED

Your countings and corresponding normalised results are reported below.

Slide Ref. : D	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15
Results F/mm ²	60	448	162	359	113	185	32	78	412	133	866	91	201	388	243
Norm. Results	0.64	1.36	1.03	1.55	0.75	1.03	0.41	0.84	1.43	1.14	1.93	1.50	1.30	1.34	1.34

Normalised Mean : 1.17
Coefficient of Variation : 33.8

Your individual position is plotted on the following diagram:

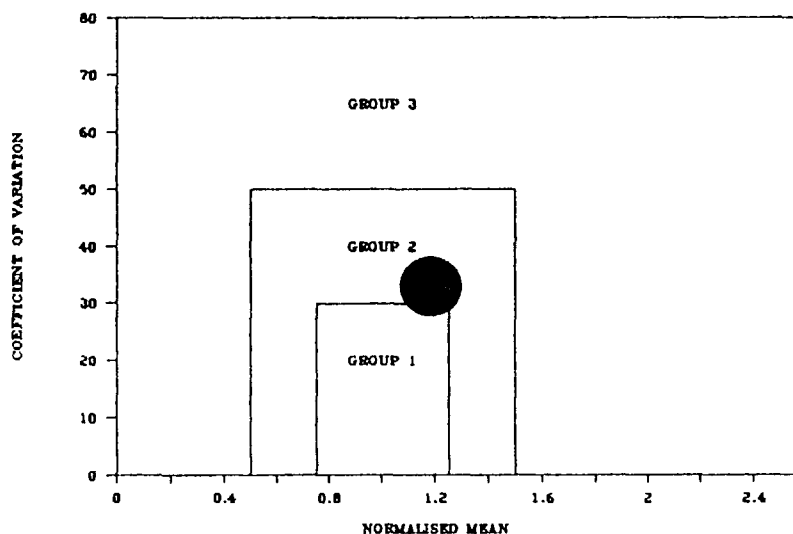

Group 1 : Counters with normalised mean in the range
0,75 - 1,25 and coefficient of variation below 30 %

Group 2 : Counters with normalised mean in the range
0,5 - 1,5 and coefficient of variation below 50 %

Group 3 : Counters with normalised mean outside the range
0,5 - 1,5 or coefficient of variation above 50 %

CTD026255

A.I.A. - FIBRE COUNTING TRIAL - 1990

PROVISIONAL POSITION DATA SHEET


Name : Mrs Laura SHEMANSKI
Company : CERTAINTEED

Your countings and corresponding normalised results are reported below.

Slide Ref. : D	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15
Results F/mm ²	87	270	129	232	124	191	82	66	260	67	404	50	201	339	175
Norm. Results	0.93	0.82	0.82	1.00	0.82	1.06	1.04	0.71	0.90	0.57	0.90	0.82	1.30	1.17	0.97

Normalised Mean : 0.92
Coefficient of Variation : 19.5

Your individual position is plotted on the following diagram:

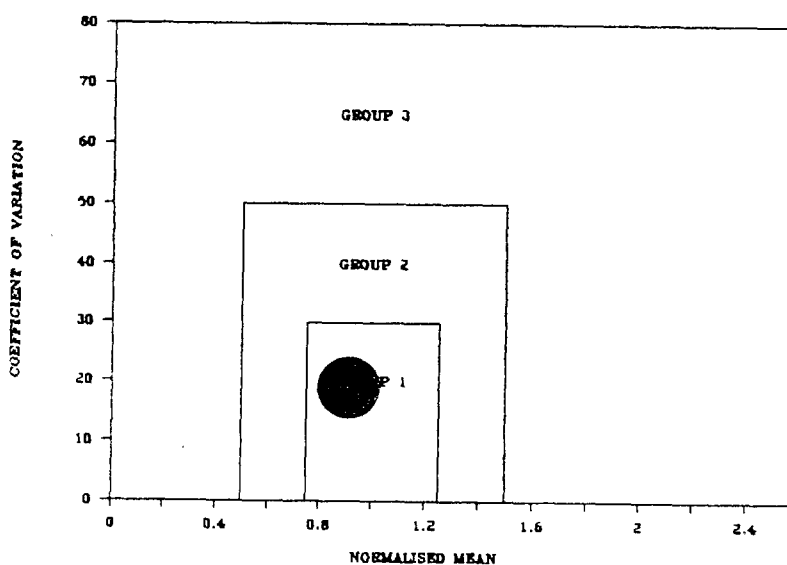

Group 1 : Counters with normalised mean in the range
0,75 - 1,25 and coefficient of variation below 30 %

Group 2 : Counters with normalised mean in the range
0,5 - 1,5 and coefficient of variation below 50 %

Group 3 : Counters with normalised mean outside the range
0,5 - 1,5 or coefficient of variation above 50 %