

A-105

MEASUREMENT AND CONTROL
OF ASBESTOS DUST EXPOSURE

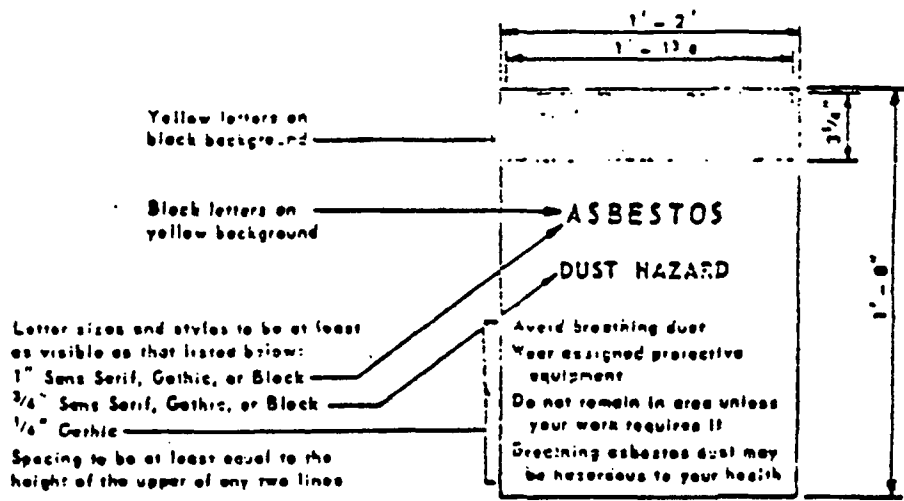


FIGURE 1 - CAUTION SIGN - ASBESTOS DUST

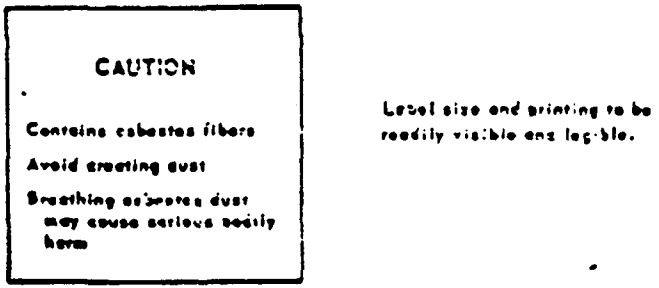


FIGURE 2 - TYPICAL CAUTION LABEL

Figures 1 and 2 meet OSHA requirements, 29 CFR 1910.103.

DUP 0902949

120914