



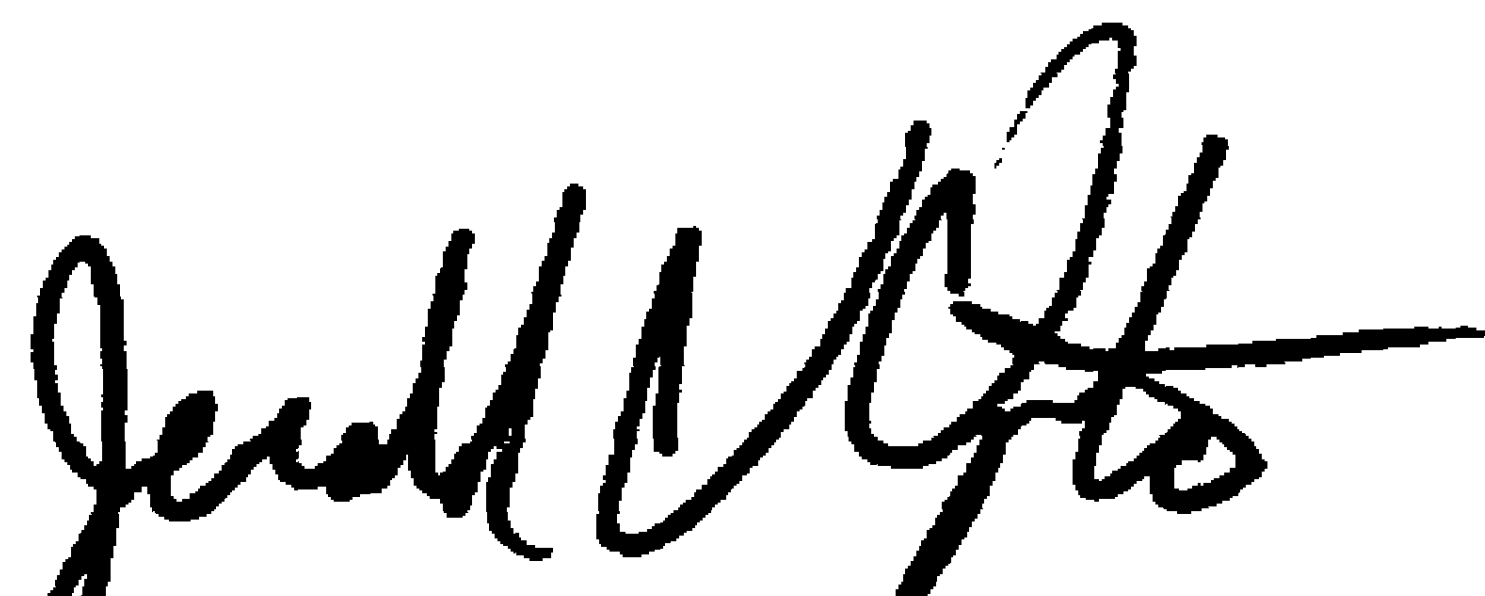
A

Interoffice Communication

To : A. H. Sather
From : J. V. Uptain
Date : June 10, 1980
Subject : VCM DOSIMETRY - MAY, 1980

Following are the results of VCM dosimetry during May. 66 samples were taken, one (1) of which indicated overexposure to a Vinyl Department Operator, who was changing filters in a recovered VCM filter pack in the new reactor area. He was wearing an air-line respirator during the task.

<u>Range</u>	<u>No.</u>	<u>%</u>
0.0-0.5	63	95.45
0.5-1.0	2	3.03
1.0-5.0	0	0
5.0+	1	1.52
	<u>66</u>	<u>100.00</u>

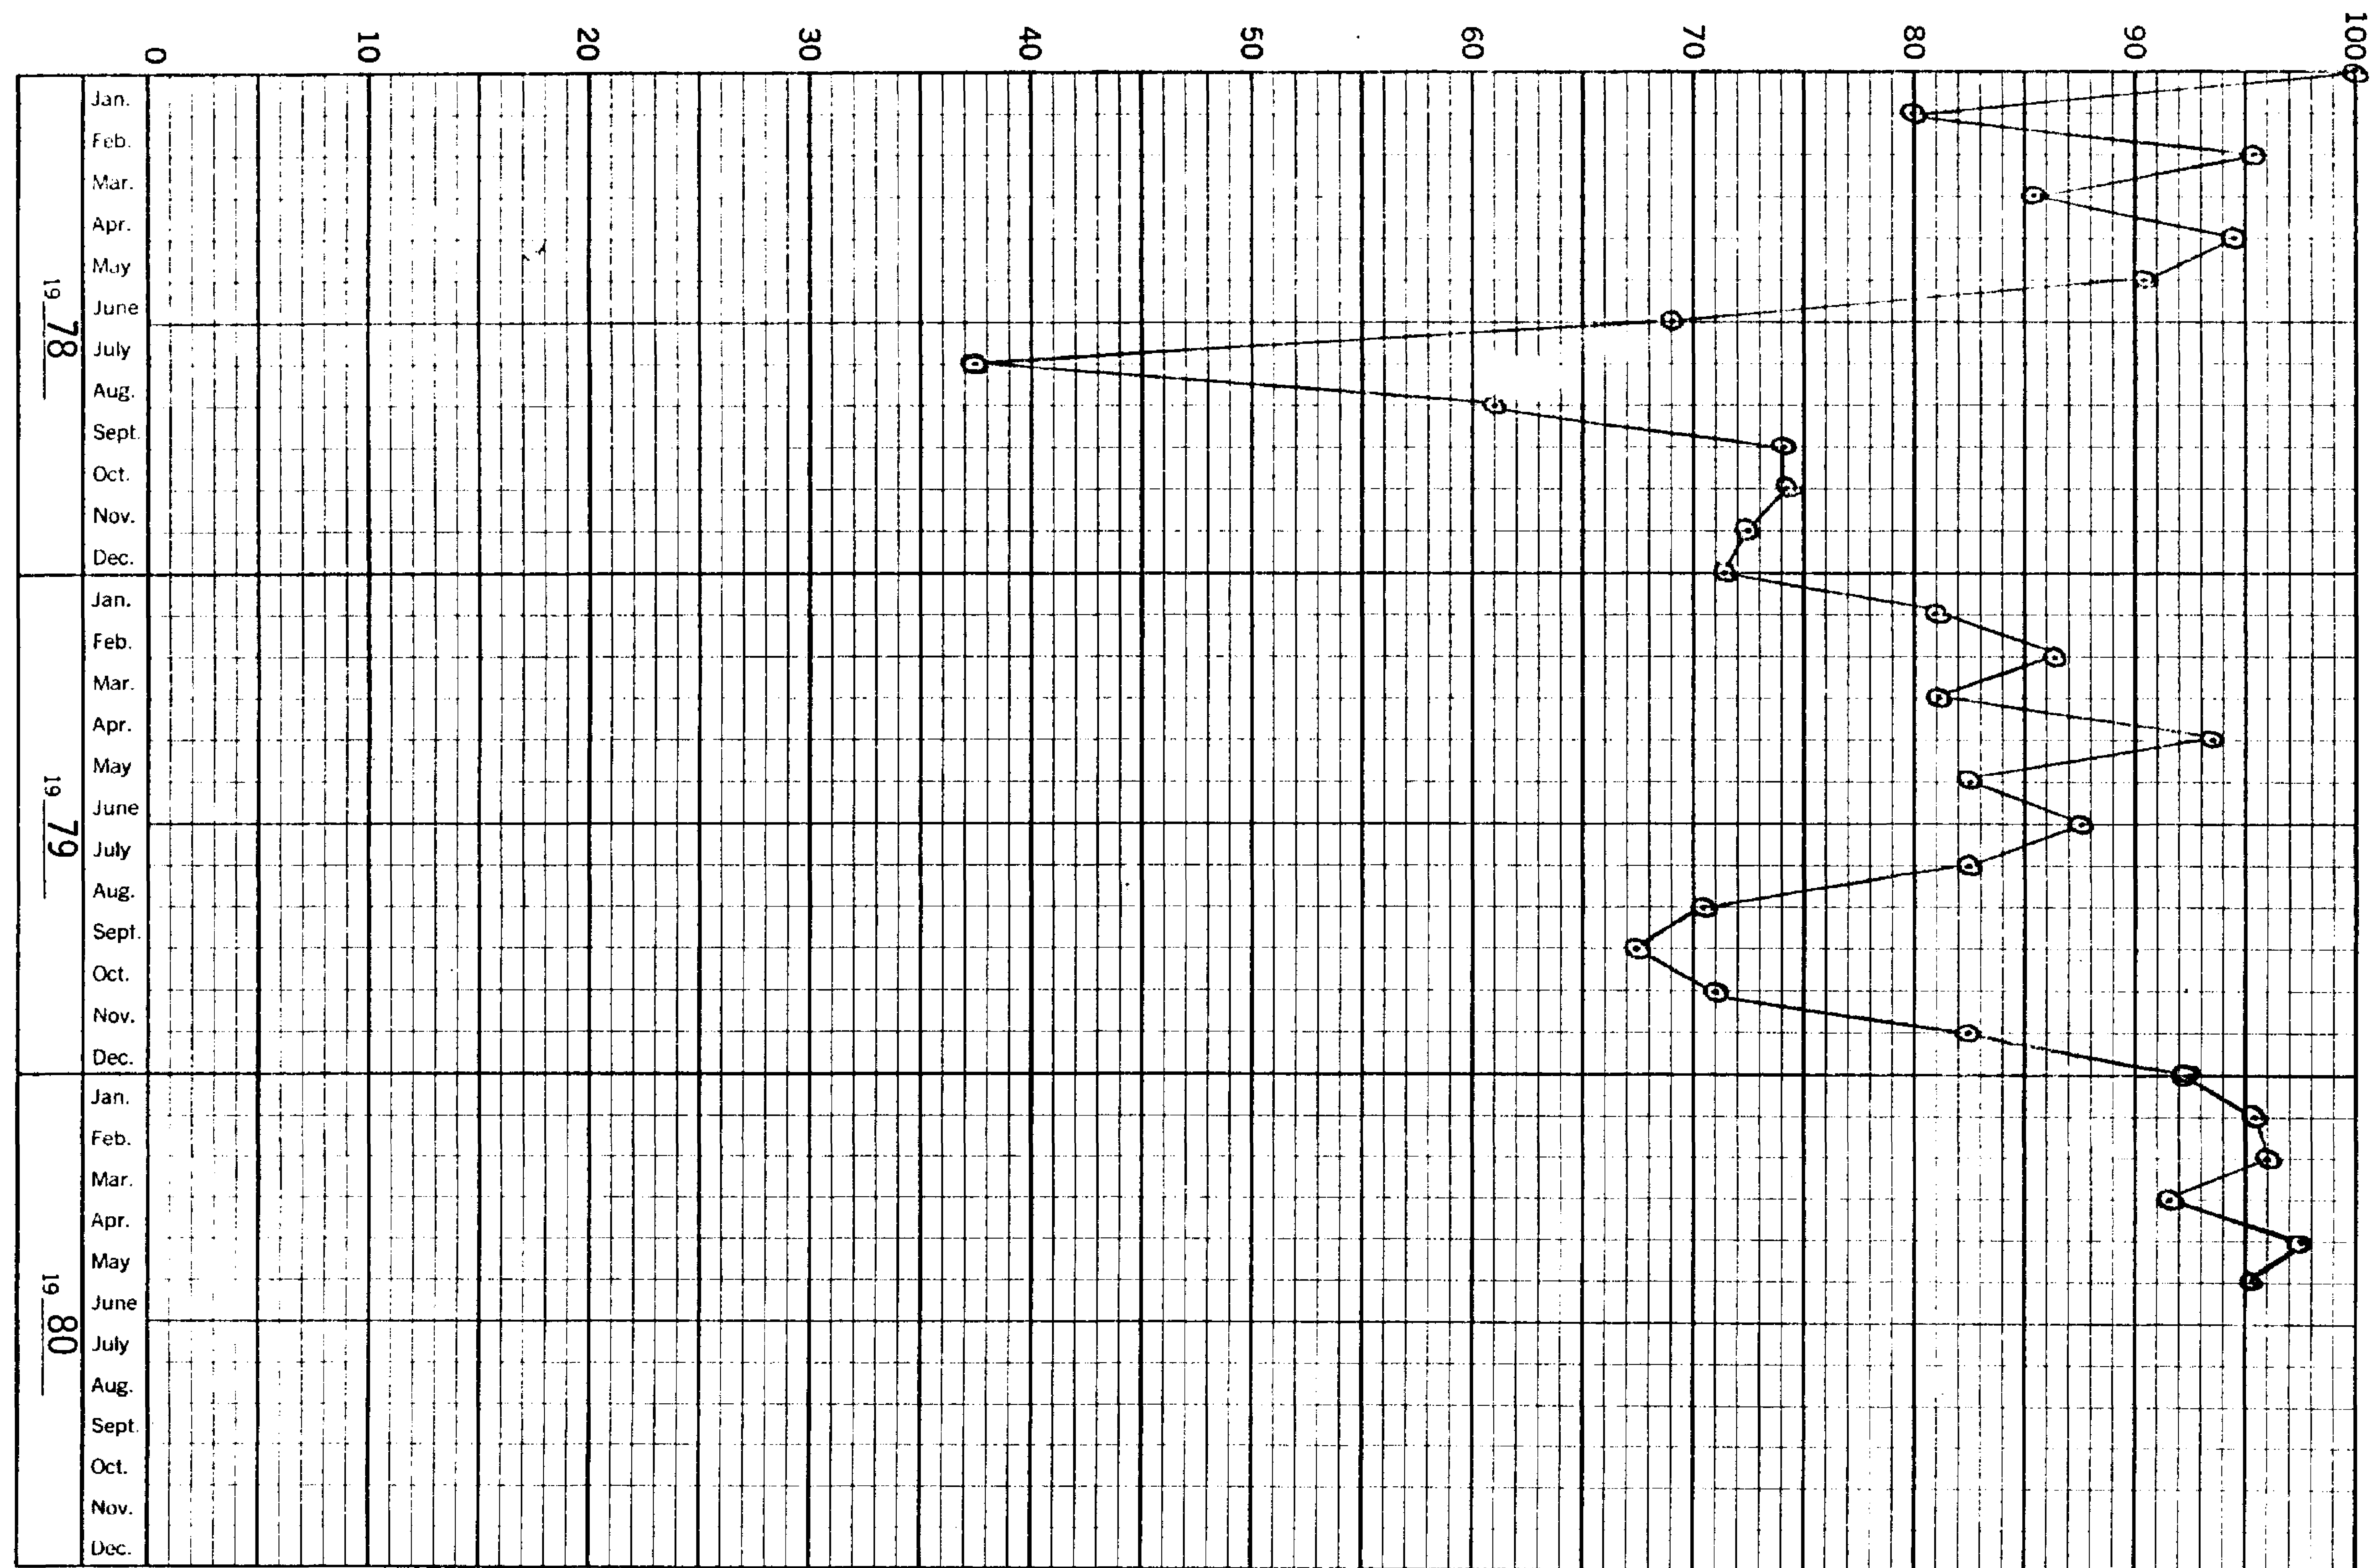

Jerald Uptain

cjt

Attachments

c: CLM, CRM, JRM, SJV, JLC, RAF, TBD, RDJ, J. J. Hall - Houston,
O. D. Steffey - Ponca City

PERCENT OF TOTAL SAMPLES LESS THAN 0.5 PPM



VCM DOSIMETRY TREND, BELOW 0.5 PPM
-ABERDEEN-

PERCENT OF TOTAL SAMPLES LESS THAN 1.0 PPM

