

# Federal Register

SATURDAY, MARCH 25, 1972  
WASHINGTON, D.C.

Volume 37 ■ Number 59

PART II



PLAINTIFF'S EXHIBIT

CAP-893

## DEPARTMENT OF THE INTERIOR

Bureau of Mines

■

Respiratory Protective Devices;  
Tests for Permissibility; Fees

## Title 30—MINERAL RESOURCES

### Chapter I—Bureau of Mines, Department of the Interior

#### SUBCHAPTER B—RESPIRATORY PROTECTIVE APPARATUS; TESTS FOR PERMISSIBILITY; FEES

#### PART 11—RESPIRATORY PROTECTIVE DEVICES; TESTS FOR PERMISSIBILITY; FEES

##### PART 12—SUPPLIED-AIR RESPIRATORS

##### PART 13—GAS MASKS

#### PART 14—FILTER-TYPE DUST, FUME, AND MIST RESPIRATORS

#### PART 14a—NONEMERGENCY GAS RESPIRATORS (CHEMICAL CARTRIDGE RESPIRATORS, INCLUDING PAINT SPRAY RESPIRATORS)

Pursuant to the authority vested in the Secretary of the Interior under 36 Stat. 369, as amended 37 Stat. 681 (30 U.S.C. 3, 5, and 7), and the authority vested in the Secretary of the Interior and the Secretary of Health, Education, and Welfare under sections 202(h), 204, and 508 of the Federal Coal Mine Health and Safety Act of 1969 (30 U.S.C. 842(h), 844, and 957), there was published in the *FEDERAL REGISTER* for March 10, 1971 (36 F.R. 4652) a notice of proposed rule making wherein it was proposed to revoke Parts 11, 12, 13, 14, and 14a of Subchapter B, Chapter I, Title 30, Code of Federal Regulations (Bureau of Mines Schedules 13E, 14F, 19B, 21B, and 23B), and to substitute therefor a new Part 11, prescribing the approval procedures, establishing the fees, and consolidating and extending the requirements for obtaining joint approval of respirators by the Bureau of Mines, Department of the Interior and the National Institute for Occupational Safety and Health, Department of Health, Education, and Welfare.

Interested persons were afforded a period of 45 days from the date of publication of the notice within which to submit written comments, suggestions, or objections to the proposed amendments. Approximately 15 associations, companies, labor organizations, individuals, and State and Federal agencies submitted comments, suggestions, or objections. In addition interested parties informally conferred with officials of the Department of the Interior and the Department of Health, Education, and Welfare in March, April, October, and November 1971 in order to discuss the proposed amendments.

Some of the regulations have been revised as suggested; in other instances revisions have been made in view of the comments received.

The proposed regulations specified that protection factors for certain types of respirators would be determined by the Bureau during the course of testing. A suggestion was received that protection factors be determined for all types of respirators. After thorough consideration of this issue, the Bureau and the

Institute have decided that although the concept of protection factors is valid, present technology in this area is insufficient to produce reliable data upon which to base such factors. Therefore, references to protection factors have been deleted from the regulations, with a view toward working to improve relevant technology and data in order to incorporate requirements for protection factors into Part 11 at a later date.

Other significant technical revisions are: (1) Performance requirements have replaced certain design specifications; and (2) tests have been included for powered air-purifying respirators. Certain procedural revisions have also been made. The arrangement and numbering system of the proposed amendments has been totally redesignated so as to place all procedural requirements at the beginning of Part 11 (Subparts A through F), followed by all technical requirements (Subparts G through M). Expanded and more stringent quality control requirements have been established (Subpart E); Examples of causes which may result in revocation of the certificate of approval have been specified. The time limit for phasing out respirators approved under revoked Parts 11, 12, 13, 14, and 14a of this Title 30 has been clarified (see § 11.2).

A suggestion was received that models submitted for testing and approval be made only on regular production tooling with no operations included which would not be incorporated in regular production processing in order to insure that commercially produced respirators would be identical in all respects to those tested and approved under these regulations. This suggestion was carefully considered. However, it was determined by the Bureau and the Institute that such a requirement might well operate to obstruct advances in respirator technology, since substantial investment would be necessary to build production models with no adequate assurance of ultimate approval. Consequently it was decided to continue the testing of soundly designed and constructed prototype models; however, upon completion of such testing the Bureau and the Institute may require the applicant to resubmit a production model for additional testing prior to issuance of a certificate of approval (see §§ 11.11 (e) and 11.30).

Subchapter B of Chapter I, Title 30, Code of Federal Regulations, amended by revoking Parts 11, 12, 13, 14, and 14a, and substituting therefor a new Part 11—Respiratory Protective Devices; Tests for Permissibility; Fees, as set forth below is herewith promulgated and shall become effective 60 days following publication in the *FEDERAL REGISTER*.

W. T. PECORA,  
*Acting Secretary of the Interior.*  
FEBRUARY 17, 1972.

ELLIOT L. RICHARDSON,  
*Secretary of Health,  
Education, and Welfare.*  
MARCH 10, 1972.

|        |                                                                                                                                                            |
|--------|------------------------------------------------------------------------------------------------------------------------------------------------------------|
|        | Subpart A—General Provisions                                                                                                                               |
| Sec.   |                                                                                                                                                            |
| 11.1   | Purpose.                                                                                                                                                   |
| 11.2   | Approved respirators.                                                                                                                                      |
| 11.2-1 | Selection, fit, use, and maintenance of approved respirators.                                                                                              |
| 1.3    | Definitions.                                                                                                                                               |
| 1.4    | Incorporation by reference.                                                                                                                                |
|        | Subpart B—Application for Approval                                                                                                                         |
| 11.10  | Application procedures.                                                                                                                                    |
| 11.11  | Contents of application.                                                                                                                                   |
| 11.12  | Delivery of respirators by applicant; requirements.                                                                                                        |
|        | Subpart C—Fees                                                                                                                                             |
| 11.20  | Examination, inspection, and testing of complete respirator assemblies; fees.                                                                              |
| 11.21  | Examination, inspection, and testing of respirator components or subassemblies; fees.                                                                      |
| 11.22  | Unlisted fees; additional fees; payment by applicant prior to approval.                                                                                    |
|        | Subpart D—Approval and Disapproval                                                                                                                         |
| 11.30  | Certificates of approval; scope of approval.                                                                                                               |
| 11.31  | Certificates of approval; contents.                                                                                                                        |
| 11.32  | Notice of disapproval.                                                                                                                                     |
| 11.33  | Approval labels and markings; approval of contents; use.                                                                                                   |
| 11.34  | Revocation of certificates of approval.                                                                                                                    |
| 11.35  | Changes or modifications of approved respirators; issuance of modification of certificate of approval.                                                     |
| 11.36  | Delivery of changed or modified approved respirator.                                                                                                       |
|        | Subpart E—Quality Control                                                                                                                                  |
| 11.40  | Quality control plans; filing requirements.                                                                                                                |
| 11.41  | Quality control plans; contents.                                                                                                                           |
| 11.42  | Proposed quality control plans; approval by the Bureau and the Institute.                                                                                  |
| 11.43  | Quality control records; review by the Bureau and the Institute; revocation of approval.                                                                   |
|        | Subpart F—Classification of Approved Respirators; Scope of Approval; Atmospheric Hazards; Service Time                                                     |
| 11.50  | Types of respirators to be approved; scope of approval.                                                                                                    |
| 11.51  | Entry and escape, or escape only; classification.                                                                                                          |
| 11.52  | Respiratory hazards; classification.                                                                                                                       |
| 11.53  | Service time; classification.                                                                                                                              |
|        | Subpart G—General Construction and Performance Requirements                                                                                                |
| 11.60  | Construction and performance requirements; general.                                                                                                        |
| 11.61  | General construction requirements.                                                                                                                         |
| 11.62  | Component parts; minimum requirements.                                                                                                                     |
| 11.63  | Test requirements; general.                                                                                                                                |
| 11.64  | Pretesting by applicant; approval of test methods by the Bureau.                                                                                           |
| 11.65  | Conduct of examinations, inspections, and tests by the Bureau and the Institute; assistance by applicant; observers; recorded data; public demonstrations. |
| 11.66  | Withdrawal of applications; refund of fees.                                                                                                                |

Subpart H—Self-Contained Breathing Apparatus

| Sec.                |                                                                                                        |
|---------------------|--------------------------------------------------------------------------------------------------------|
| 11.70               | Self-contained breathing apparatus; description.                                                       |
| 11.71               | Self-contained breathing apparatus; required components.                                               |
| 11.72               | Breathing tubes; minimum requirements.                                                                 |
| 11.73               | Harnesses; installation and construction; minimum requirements.                                        |
| 11.74               | Apparatus containers; minimum requirements.                                                            |
| 11.75               | Half-mask facepieces, full facepieces, mouthpieces; fit; minimum requirements.                         |
| 11.76               | Facepieces; eyepieces; minimum requirements.                                                           |
| 11.77               | Inhalation and exhalation valves; minimum requirements.                                                |
| 11.78               | Head harnesses; minimum requirements.                                                                  |
| 11.79               | Breathing gas; minimum requirements.                                                                   |
| 11.79-1             | Interchangeability of oxygen and air prohibited.                                                       |
| 11.80               | Compressed breathing gas and liquefied breathing gas containers; minimum requirements.                 |
| 11.81               | Gas pressure gages; minimum requirements.                                                              |
| 11.82               | Timers; elapsed time indicators; remaining service life indicators; minimum requirements.              |
| 11.83               | Hand-operated valves; minimum requirements.                                                            |
| 11.84               | Breathing bags; minimum requirements.                                                                  |
| 11.85               | Self-contained breathing apparatus; performance requirements; general.                                 |
| 11.85-1             | Component parts exposed to oxygen pressures; minimum requirements.                                     |
| 11.85-2             | Compressed gas filters; minimum requirements.                                                          |
| 11.85-3             | Breathing bag test.                                                                                    |
| 11.85-4             | Weight requirement.                                                                                    |
| 11.85-5             | Breathing resistance test; inhalation.                                                                 |
| 11.85-6             | Breathing resistance test; exhalation.                                                                 |
| 11.85-7             | Exhalation valve leakage test.                                                                         |
| 11.85-8             | Gas flow test; open-circuit apparatus.                                                                 |
| 11.85-9             | Gas flow test; closed-circuit apparatus.                                                               |
| 11.85-10            | Service time test; open-circuit apparatus.                                                             |
| 11.85-11            | Service time test; closed-circuit apparatus.                                                           |
| 11.85-12            | Test for carbon dioxide in inspired gas; open- and closed-circuit apparatus; maximum allowable limits. |
| 11.85-13            | Tests during low temperature operation.                                                                |
| 11.85-14            | Man tests; testing conditions; general requirements.                                                   |
| 11.85-15            | Man tests 1, 2, 3, and 4; requirements.                                                                |
| 11.85-16            | Man test 5; requirements.                                                                              |
| 11.85-17            | Man test 6; requirements.                                                                              |
| 11.85-18            | Man tests; performance requirements.                                                                   |
| 11.85-19            | Gas tightness test; minimum requirements.                                                              |
| Subpart I—Gas Masks |                                                                                                        |
| 11.90               | Gas masks; description.                                                                                |
| 11.91               | Gas masks; required components.                                                                        |
| 11.92               | Canisters and cartridges in parallel; resistance requirements.                                         |
| 11.93               | Canisters and cartridges; color and markings; requirements.                                            |
| 11.94               | Filters used with canisters and cartridges; location; replacement.                                     |

| Sec.     |                                                                                        |
|----------|----------------------------------------------------------------------------------------|
| 11.95    | Breathing tubes; minimum requirements.                                                 |
| 11.96    | Harnesses; installation and construction; minimum requirements.                        |
| 11.97    | Gas mask containers; minimum requirements.                                             |
| 11.98    | Half-mask facepieces, full facepieces, and mouthpieces; fit; minimum requirements.     |
| 11.99    | Facepieces; eyepieces; minimum requirements.                                           |
| 11.100   | Inhalation and exhalation valves; minimum requirements.                                |
| 11.101   | Head harnesses; minimum requirements.                                                  |
| 11.102   | Gas masks; performance requirements; general.                                          |
| 11.102-1 | Breathing resistance test; minimum requirements.                                       |
| 11.102-2 | Exhalation valve leakage test.                                                         |
| 11.102-3 | Facepiece tests; minimum requirements.                                                 |
| 11.102-4 | Dust, fume, mist, and smoke tests; canisters containing filters; minimum requirements. |
| 11.102-5 | Canister bench tests; minimum requirements.                                            |

Subpart J—Supplied-Air Respirators

| Sec.     |                                                                                                                      |
|----------|----------------------------------------------------------------------------------------------------------------------|
| 11.110   | Supplied-air respirators; description.                                                                               |
| 11.111   | Supplied-air respirators; required components.                                                                       |
| 11.112   | Breathing tubes; minimum requirements.                                                                               |
| 11.113   | Harnesses; installation and construction; minimum requirements.                                                      |
| 11.114   | Respirator containers; minimum requirements.                                                                         |
| 11.115   | Half-mask facepieces, full facepieces, hoods, and helmets; fit; minimum requirements.                                |
| 11.116   | Facepieces, hoods, and helmets; eyepieces; minimum requirements.                                                     |
| 11.117   | Inhalation and exhalation valves; check valves; minimum requirements.                                                |
| 11.118   | Head harnesses; minimum requirements.                                                                                |
| 11.119   | Head and neck protection; supplied-air respirators; minimum requirements.                                            |
| 11.120   | Air velocity and noise levels; hoods and helmets; minimum requirements.                                              |
| 11.121   | Breathing gas; minimum requirements.                                                                                 |
| 11.122   | Air supply source; hand-operated or motor driven air blowers; Type A supplied-air respirators; minimum requirements. |
| 11.123   | Terminal fittings or chambers; Type B supplied-air respirators; minimum requirements.                                |
| 11.124   | Supplied-air respirators; performance requirements; general.                                                         |
| 11.124-1 | Hand-operated blower test; minimum requirements.                                                                     |
| 11.124-2 | Motor-operated blower test; minimum requirements.                                                                    |
| 11.124-3 | Method of measuring the power and torque required to operate blowers.                                                |
| 11.124-4 | Type B supplied-air respirator; minimum requirements.                                                                |
| 11.124-5 | Type C supplied-air respirator, continuous flow class; minimum requirements.                                         |
| 11.124-6 | Type C supplied-air respirator, demand and pressure demand class; minimum requirements.                              |
| 11.124-7 | Air-supply line tests; minimum requirements.                                                                         |
| 11.124-8 | Harness test; minimum requirements.                                                                                  |

| Sec.      |                                                                                                                                           |
|-----------|-------------------------------------------------------------------------------------------------------------------------------------------|
| 11.124-9  | Breathing tube test; minimum requirements.                                                                                                |
| 11.124-10 | Airflow resistance test, Type A and Type AE supplied-air respirators; minimum requirements.                                               |
| 11.124-11 | Airflow resistance test; Type B and Type BE supplied-air respirators; minimum requirements.                                               |
| 11.124-12 | Airflow resistance test; Type C supplied-air respirator, continuous flow class and Type CE supplied-air respirator; minimum requirements. |
| 11.124-13 | Airflow resistance test; Type C supplied-air respirator, demand class; minimum requirements.                                              |
| 11.124-14 | Airflow resistance test; Type C supplied-air respirator, pressure-demand class; minimum requirements.                                     |
| 11.124-15 | Exhalation valve leakage test.                                                                                                            |
| 11.124-16 | Man tests for gases and vapors supplied-air respirators; general performance requirements.                                                |
| 11.124-17 | Man tests for gases and vapors; Type A and Type AE respirators; test requirements.                                                        |
| 11.124-18 | Man tests for gases and vapors; Type B and Type BE respirators; test requirements.                                                        |
| 11.124-19 | Man test for gases and vapors; Type C respirators, continuous-flow class and Type CE supplied-air respirators; test requirements.         |
| 11.124-20 | Man test for gases and vapors; Type C supplied-air respirators, demand and pressure-demand classes; test requirements.                    |
| 11.124-21 | Tests for protection during abrasive blasting; Type AE, Type BE, and Type CE supplied-air respirators; general performance requirements.  |
| 11.124-22 | Test for protection during abrasive blasting; Type AE supplied-air respirator; test requirements.                                         |
| 11.124-23 | Test for protection during abrasive blasting; Type BE supplied-air respirator; test requirements.                                         |
| 11.124-24 | Test for protection during abrasive blasting; Type CE supplied-air respirator; test requirements.                                         |

Subpart K—Dust, Fume, and Mist Respirators

| Sec.   |                                                                                                    |
|--------|----------------------------------------------------------------------------------------------------|
| 11.130 | Dust, fume, and mist respirators; description.                                                     |
| 11.131 | Dust, fume and mist respirators; required components.                                              |
| 11.132 | Breathing tubes; minimum requirements.                                                             |
| 11.133 | Harnesses; installation and construction; minimum requirements.                                    |
| 11.134 | Respirator containers; minimum requirements.                                                       |
| 11.135 | Half-mask facepieces, full facepieces, hoods, helmets, and mouthpieces; fit; minimum requirements. |
| 11.136 | Facepieces, hoods, and helmets; eyepieces; minimum requirements.                                   |
| 11.137 | Inhalation and exhalation valves; minimum requirements.                                            |
| 11.138 | Head harnesses; minimum requirements.                                                              |
| 11.139 | Air velocity and noise levels; hoods and helmets; minimum requirements.                            |
| 11.140 | Dust, fume, and mist respirators; performance requirements; general.                               |

- Sec.  
11.140-1 Isoamyl acetate tightness test; dust, fume, and mist respirators designed for respiratory protection against fumes of various metals having an air contamination level not less than 0.05 milligram per cubic meter; minimum requirements.
- 11.140-2 Isoamyl acetate tightness test; respirators designed for respiratory protection against dusts, fumes, and mists having an air contamination level less than 0.05 milligram per cubic meter, or against radionuclides; minimum requirements.
- 11.140-3 Air-purifying filter tests; performance requirements; general.
- 11.140-4 Silica dust test; single-use or reusable filters; minimum requirements.
- 11.140-5 Silica dust test; single-use dust respirators; minimum requirements.
- 11.140-6 Lead fume test; minimum requirements.
- 11.140-7 Silica mist test; minimum requirements.
- 11.140-8 Tests for respirators designed for respiratory protection against more than one type of dispersed; minimum requirements.
- 11.140-9 Airflow resistance tests; all dust, fume, and mist respirators; minimum requirements.
- 11.140-10 Exhalation valve leakage test; minimum requirements.
- 11.140-11 DOP filter test; respirators designed as respiratory protection against dusts, fumes, and mists having an air contamination level less than 0.05 milligram per cubic meter and against radionuclides; minimum requirements.
- 11.140-12 Silica dust loading test; respirators designed as protection against dusts, fumes, and mists having an air contamination level less than 0.05 milligram per cubic meter and against radionuclides; minimum requirements.
- Subpart I—Chemical Cartridge Respirators**
- 11.150 Chemical cartridge respirators; description.
- 11.151 Chemical cartridge respirators; required components.
- 11.152 Cartridges in parallel; resistance requirements.
- 11.153 Cartridges; color and markings; requirements.
- 11.154 Filters used with chemical cartridges; location; replacement.
- 11.155 Breathing tubes; minimum requirements.
- 11.156 Harnesses; installation and construction; minimum requirements.
- 11.157 Respirator containers; minimum requirements.
- 11.158 Half-mask facepieces, full facepieces, mouthpieces, hoods, and helmets; fit; minimum requirements.
- 11.158-1 Facepieces, hoods, and helmets; eyepieces; minimum requirements.
- 11.159 Inhalation and exhalation valves; minimum requirements.
- 11.160 Head harnesses; minimum requirements.
- 11.161 Air velocity and noise levels; hoods and helmets; minimum requirements.

- Sec.  
11.162 Chemical cartridge respirators; performance requirements; general.
- 11.162-1 Breathing resistance test; minimum requirements.
- 11.162-2 Exhalation valve leakage test; minimum requirements.
- 11.162-3 Facepiece test; minimum requirements.
- 11.162-4 Lacquer and enamel mist tests; respirators with filters; minimum requirements; general.
- 11.162-5 Lacquer mist test; minimum requirements.
- 11.162-6 Enamel mist test; minimum requirements.
- 11.162-7 Dust, fume, and mist tests; respirators with filters; minimum requirements; general.
- 11.162-8 Bench tests; gas and vapor tests; minimum requirements; general.

#### Subpart M—Pesticide Respirators

- 11.170 Pesticide respirators; description.
- 11.171 Pesticide respirators; required components.
- 11.172 Canisters and cartridges in parallel; resistance requirements.
- 11.173 Canisters and cartridges; color and markings; requirements.
- 11.174 Filters used with canisters and cartridges; location; replacement.
- 11.175 Breathing tubes; minimum requirements.
- 11.176 Harnesses; installation and construction; minimum requirements.
- 11.177 Respirator containers; minimum requirements.
- 11.178 Half-mask facepieces, full facepieces, hoods and helmets, and mouthpieces; fit; minimum requirements.
- 11.179 Facepieces, hoods and helmets; eyepieces; minimum requirements.
- 11.180 Inhalation and exhalation valves; minimum requirements.
- 11.181 Head harnesses; minimum requirements.
- 11.182 Air velocity and noise levels; hoods and helmets; minimum requirements.
- 11.183 Pesticide respirators; performance requirements; general.
- 11.183-1 Breathing resistance test; minimum requirements.
- 11.183-2 Exhalation valve leakage test; minimum requirements.
- 11.183-3 Facepiece test; minimum requirements.
- 11.183-4 Silica dust test; minimum requirements.
- 11.183-5 Lead fume test; minimum requirements.
- 11.183-6 Dioctyl-phthalate test; minimum requirements.
- 11.183-7 Bench tests; minimum requirements.

**AUTHORITY:** The provisions of this Part 11 issued under sections 202(h), 204, and 508 of the Federal Coal Mine Health and Safety Act of 1969 (30 U.S.C. 842(h), 844, and 957) and 38 Stat. 369, as amended 37 Stat. 681 (30 U.S.C. 3, 6, and 7).

#### Subpart A—General Provisions

##### § 11.1 Purpose.

The purpose of the regulations contained in this Part 11 is: (a) To establish procedures and prescribe requirements which must be met in filing applications for joint approval by the Bureau of Mines

and the National Institute for Occupational Safety and Health of respirators or changes or modifications of approved respirators; (b) to establish a schedule of fees to be charged each applicant for the inspections, examinations, and testing conducted by the Bureau under the provisions of this part; (c) to provide for the issuance of certificates of approval or modifications of certificates of approval for respirators which have met the applicable construction, performance, and respiratory protection requirements set forth in this part; and (d) to specify minimum requirements and to prescribe methods to be employed by the Bureau and by the applicant in conducting inspections, examinations, and tests to determine the effectiveness of respirators used during entry into or escape from hazardous atmospheres.

##### § 11.2 Approved respirators.

(a) Until March 30, 1974, respirators or combinations of respirators shall be considered to be approved for use during entry into hazardous mine atmospheres, escape from hazardous mine atmospheres, or both, where such respirators or combinations of respirators are: (1) The same in all respects as those respirators which have been approved after meeting the minimum requirements for performance and respiratory protection set forth in this Part 11; or (2) fabricated, assembled, or built under any approval, or any modification thereof, issued by the U.S. Bureau of Mines, Department of the Interior, in accordance with the schedules set forth below; and (3) maintained in an approved condition:

(i) Self-contained Breathing Apparatus, Bureau of Mines Schedules 13, March 5, 1919; 13A, January 21, 1930; 13B, August 12, 1935; 13C, July 9, 1946; 13D, September 22, 1956; and 13E, July 19, 1968.

(ii) Gas Masks, Bureau of Mines Schedule 14F, April 23, 1955.

(iii) Supplied-air Respirators, Bureau of Mines Schedule 19B, April 19, 1955.

(iv) Filter-type Dust, Fume, and Mist Respirators, Bureau of Mines Schedule 21B, January 19, 1965.

(v) Nonemergency Gas Respirators, Bureau of Mines Schedule 23B, August 4, 1959.

(b) After March 30, 1974, respirators or combinations of respirators shall be considered to be approved for use during entry into hazardous mine atmospheres, escape from hazardous mine atmospheres, or both, only where such respirators or combinations of such respirators are: (1) The same in all respects as those respirators which have been approved after meeting the minimum requirements for performance and respiratory protection prescribed in this Part 11; and (2) maintained in an approved condition.

##### § 11.2-1 Selection, fit, use, and maintenance of approved respirators.

In order to insure the maximum amount of respiratory protection, approved respirators shall be selected,

fitted, used, and maintained in accordance with the provisions of the American National Standard Practices for Respiratory Protection, Z88.2, obtainable from American National Standards Institute, Inc., 1430 Broadway, New York, NY 10018.

### § 11.3 Definitions.

As used in this part—

(a) "Air Contamination Level" means the standards of contaminant levels prescribed by the Secretary of Labor in accordance with the provisions of the Occupational Safety and Health Act of 1970 (Public Law 91-596; 84 Stat. 1590).

(b) "Applicant" means an individual, partnership, company, corporation, association, or other organization that designs, manufactures, assembles, or controls the assembly of a respirator and who seeks to obtain a certificate of approval for such respirator.

(c) "Approval" means a certificate or formal document issued by the Bureau and the Institute stating that an individual respirator or combination of respirators has met the minimum requirements of this Part 11, and that the applicant is authorized to use and attach an approval label to any respirator, respirator container, or instruction card for any respirator manufactured or assembled in conformance with the plans and specifications upon which the approval was based, as evidence of such approval.

(d) "Approved" means conforming to the minimum requirements of this Part 11.

(e) "Auxiliary equipment" means a self-contained breathing apparatus, the use of which is limited in underground mine rescue and recovery operations to situations where the wearer has ready access to fresh air and at least one crew equipped with approved self-contained breathing apparatus of 2 hours or longer rating, is in reserve at a fresh-air base.

(f) "Bureau" means the U.S. Bureau of Mines, Department of the Interior.

(g) "Compressed breathing gas" means oxygen or air stored in a compressed state and supplied to the wearer in gaseous form.

(h) "Concentration limits for radionuclides" means the concentration limits set forth in Appendix B, Table 1, Column I of Title 10 CFR Part 20, by the Atomic Energy Commission.

(i) "dBA" means sound pressure levels in decibels, as measured with the A-weighted network of a standard sound level meter using slow response.

(j) "DOP" means a homogeneous liquid aerosol, having a particle diameter of 0.3 micrometer, which is generated by vaporization and condensation of dioctyl phthalate.

(k) "Dust" means a solid mechanically produced particle with a size ranging from submicroscopic to microscopic.

(l) "Respirators 'for entry into and escape from'" means respiratory devices providing protection during entry into and escape from hazardous atmospheres.

(m) "Respirators 'for escape only'" means respiratory devices providing protection only during escape from hazardous atmospheres.

(n) A "facepiece" or "mouthpiece" is a respirator component designed to provide a gas-tight or dust-tight fit with the face and may include headbands, valves, and connections for canisters, cartridges, filters, or respirable gas source.

(o) "Final inspection" means that activity carried out on a product after all manufacturing and assembly operations are completed to insure completeness and adherence to performance or other specifications, including satisfactory appearance.

(p) "Fume" means a solid condensation particle, generally less than 1 micrometer in diameter.

(q) "Gas" means an aeriform fluid which is in a gaseous state at ordinary temperature and pressure.

(r) "Hazardous atmosphere" means: (1) Any atmosphere containing a toxic or disease producing gas, vapor, dust, fume, mist, or pesticide, either immediately or not immediately dangerous to life or health; or (2) any oxygen-deficient atmosphere.

(s) A "hood" or "helmet" is a respirator component which covers the wearer's head and neck, or head, neck, and shoulders, and is supplied with incoming respirable air for the wearer to breathe. It may include a headharness and connection for a breathing tube.

(t) "Immediately dangerous to life or health" means conditions that pose an immediate threat to life or health or conditions that pose an immediate threat of severe exposure to contaminants, such as radioactive materials, which are likely to have adverse cumulative or delayed effects on health.

(u) "Incoming inspection" means the activity of receiving, examining, and accepting only those materials and parts whose quality conforms to specification requirements.

(v) "In-process inspection" means the control of products at the source of production and at each step of the manufacturing process, so that departures from specifications can be corrected before defective components or materials are assembled into the finished product.

(w) "Institute" means the National Institute for Occupational Safety and Health, Department of Health, Education, and Welfare.

(x) "Liquefied breathing gas" means oxygen or air stored in liquid form and supplied to the wearer in a gaseous form.

(y) "Mist" means a liquid condensation particle with a size ranging from submicroscopic to macroscopic.

(z) "Not immediately dangerous to life or health" means any hazardous atmosphere which may produce physical discomfort immediately, chronic poisoning after repeated exposure, or acute adverse physiological symptoms after prolonged exposure.

(aa) "Oxygen deficient atmosphere" means an atmosphere which contains an oxygen partial pressure of less than 148 millimeters of mercury (19.5 percent by volume at sea level).

(bb) "Pesticide" means (1) any substance or mixture of substances (including solvents and impurities) intended to prevent, destroy, repel, or mitigate any

insect, rodent, nematode, fungus, weed, or other form of plant or animal life or virus, and (2) any substance or mixture of substances (including solvents and impurities) intended for use as a plant regulator, defoliant, or desiccant, as defined in the Federal Insecticide, Fungicide, and Rodenticide Act of 1947, as amended (7 U.S.C. 135-135k), excluding fumigants which are applied as gases or vapors or in a solid or liquid form as pellets or poured liquids for subsequent release as gases or vapors.

(cc) "Powered air-purifying respirator" means a device equipped with a facepiece, hood, or helmet, breathing tube, canister, cartridge, filter, canister with filter, or cartridge with filter, and a blower.

(dd) "Radionuclide" means an atom identified by the constitution of its nucleus (specified by the number of protons Z, number of neutrons N, and energy, or, alternatively, by the atomic number Z, mass number A=(N+Z), and atomic mass) which exists for a measurable time; decays or disintegrates spontaneously, emits radiation, and results in the formation of new nuclides.

(ee) "Respirable dust" means a dust particle aerodynamically capable of reaching the terminal airways of the lung.

(ff) "Respirator" means any device designed to provide the wearer with respiratory protection against inhalation of a hazardous atmosphere.

(gg) "Smoke" means the products of incomplete combustion of organic substances in the form of solid and liquid particles and gaseous products in air, usually of sufficient concentration to perceptibly obscure vision.

(hh) "Vapor" means the gaseous state of a substance that is solid or liquid at ordinary temperature and pressure.

### § 11.4 Incorporation by reference.

In accordance with 5 U.S.C. 552(a) (1), the technical publications to which reference is made in this Part 11, and which have been prepared by organizations other than the Bureau of Mines, are hereby incorporated by reference and made a part hereof. The incorporated technical publications are available for examination at Approval and Testing, Health and Safety Technical Support Center, Bureau of Mines, 4800 Forbes Avenue, Pittsburgh, Pa. In addition, copies of the American National Standard Practices for Respiratory Protection, Z88.2, are available for examination in every Coal Mine Health and Safety District and Subdistrict Office.

### Subpart B—Application for Approval

#### § 11.10 Application procedures.

(a) Inspection, examination, and testing leading to the approval of the types of respirators classified in Subpart F of this part shall be undertaken by the Bureau only pursuant to written applications which meet the minimum requirements set forth in this Subpart B.

(b) Applications shall be submitted to Approval and Testing, Bureau of Mines, 4800 Forbes Avenue, Pittsburgh, PA

15213, and shall be accompanied by a check, bank draft, or money order in the amount specified in Subpart C of this part payable to the order of the U.S. Bureau of Mines.

(c) Except as provided in § 11.64, the examination, inspection, and testing of all respirators shall be conducted by Approval and Testing, Bureau of Mines, Pittsburgh, Pa. 15213.

(d) Applicants, manufacturers, or their representatives may visit or communicate with Approval and Testing in order to discuss the requirements for approval of any respirator or the proposed designs thereof. No charge shall be made for such consultation and no written report shall be issued to applicants, manufacturers, or their representatives by the Bureau as a result of such consultation.

#### § 11.11 Contents of application.

(a) Each application for approval shall contain a complete written description of the respirator for which approval is requested together with drawings and specifications (and lists thereof) showing full details of construction of the respirator and of the materials used. Drawings and specifications (and lists thereof) shall be submitted in triplicate.

(b) Drawings shall be titled, numbered, and dated; any revision dates shall be shown on the drawings, and the purpose of each revision being sought shall be shown on the drawing or described on an attachment to the drawing to which it applies.

(c) Each application for approval shall contain a proposed plan for quality control which meets the minimum requirements set forth in Subpart E of this part.

(d) Each application shall contain a statement that the respirator has been pretested by the applicant as prescribed in § 11.64, and shall include the results of such tests.

(e) Each application for approval shall contain a statement that the respirator and component parts submitted for approval are either (1) prototypes, or (2) made on regular production tooling, with no operation included which will not be incorporated in regular production processing.

#### § 11.12 Delivery of respirators by applicant; requirements.

(a) Each applicant shall, when an application is filed pursuant to § 11.10, be advised by the Bureau of the total number of respirators and component parts required for testing.

(b) The applicant shall deliver, at his own expense, the number of completely assembled respirators and component parts required for testing, to Approval and Testing, Bureau of Mines, Pittsburgh, Pa. 15213.

(c) Respirators and component parts submitted for approval must be made from materials specified in the application.

(d) One completely assembled respirator approved under the provisions of this part may be retained by the Bureau as a laboratory exhibit, the remaining respirators may be returned to the applicant at his own expense, upon writ-

ten request within 30 days after notice of approval. If no such request is made, the respirators will be disposed of by the Bureau in such manner as it deems appropriate.

(e) Where a respirator fails to meet the requirements for approval set forth in this part, all respirators and components delivered in accordance with this section may be returned to the applicant at his own expense, upon written request within 30 days after notice of disapproval. If no such request is made, the respirators will be disposed of by the Bureau in such manner as it deems appropriate.

#### Subpart C—Fees

##### § 11.20 Examination, inspection and testing of complete respirator assemblies; fees.

Except as provided in § 11.22, the following fees shall be charged by the Bureau for the examination, inspection and testing of complete respirator assemblies:

|                                                                                                                                                           |         |
|-----------------------------------------------------------------------------------------------------------------------------------------------------------|---------|
| (a) Self-contained breathing apparatus—                                                                                                                   |         |
| (1) Entry and escape, 1 hour or more .....                                                                                                                | \$3,500 |
| (2) Entry and escape, less than 1 hour .....                                                                                                              | 2,750   |
| (3) Escape only .....                                                                                                                                     | 2,000   |
| (b) Gas masks, including pesticide gas masks—                                                                                                             |         |
| (1) Single hazard .....                                                                                                                                   | 1,100   |
| (2) Type N .....                                                                                                                                          | 4,100   |
| (c) Supplied-air respirators .....                                                                                                                        | 750     |
| (d) Dust, fume and mist respirators—                                                                                                                      |         |
| (1) Single particulate hazard having an Air Contamination Level more than 0.05 mg./m. <sup>3</sup> or 2 million particles per cubic foot .....            | 500     |
| (2) Combination particulate hazards having an Air Contamination Level more than 0.05 mg./m. <sup>3</sup> or 2 million particles per cubic foot .....      | 750     |
| (3) Particulate hazards having an Air Contamination Level less than 0.05 mg./m. <sup>3</sup> or 2 million particles per cubic foot, radon daughters ..... | 1,250   |
| (4) All dusts, fumes and mists .....                                                                                                                      | 2,000   |
| (e) Chemical cartridge respirators .....                                                                                                                  |         |
| (f) Paint spray respirators .....                                                                                                                         | 1,600   |
| (g) Pesticide respirators .....                                                                                                                           | 1,600   |

##### § 11.21 Examination, inspection and testing of respirator components or subassemblies; fees.

Except as provided in § 11.22, the following fees shall be charged by the Bureau for the examination, inspection and testing of the individual respirator components or subassemblies:

|                      |       |
|----------------------|-------|
| (a) Facepieces ..... | \$450 |
| (b) Canisters .....  | 900   |
| (c) Cartridges ..... | 600   |
| (d) Filters .....    | 650   |
| (e) Hoses .....      | 250   |
| (f) Blowers .....    | 250   |
| (g) Harnesses .....  | 100   |

##### § 11.22 Unlisted fees; additional fees; payment by applicant prior to approval.

(a) Applications for the examination, inspection and testing of complete

respirator assemblies which are not listed in § 11.20, or for the examination, inspection, and testing of respirator components or subassemblies which are not listed in § 11.21, shall be accompanied by the following deposits:

|                                                    |         |
|----------------------------------------------------|---------|
| (1) Complete respirator assembly .....             | \$1,500 |
| (2) Each individual component or subassembly ..... | 500     |

(b) The Bureau reserves the right to conduct any examination, inspection, or test it deems necessary to determine the quality and effectiveness of any listed or unlisted respirator assembly or respirator component or subassembly, and to assess the cost of such examinations, inspections, or tests against the applicant prior to the issuance of any approval for the respiratory equipment examined, inspected, or tested.

(c) The fees charged for the examination, inspection, and testing of unlisted respirator assemblies, unlisted individual respirator components or subassemblies, and for the additional examination, inspection, and testing of listed respirator assemblies and components or subassemblies shall be at the rate of \$100 per day for each man-day required to be expended by the Bureau.

(d) Upon completion of all examinations, inspections, and tests of unlisted respirator assemblies or components, or following the completion of any additional examination, inspections, or tests of listed assemblies, or components or subassemblies, including retesting subsequent to disapproval, the Bureau shall advise the applicant in writing of the total cost assessed and the additional amount, if any, which must be paid to the Bureau as a condition of approval.

(e) In the event the amount assessed by the Bureau for unlisted assemblies, or components or subassemblies is less than the amount of the deposit submitted in accordance with paragraph (a) of this section, the Bureau shall refund the overpayment upon the issuance of any approval or notice of disapproval.

#### Subpart D—Approval and Disapproval

##### § 11.30 Certificates of approval; scope of approval.

(a) The Bureau and the Institute shall issue certificates of approval pursuant to the provisions of this subpart only for individual, completely assembled respirators which have been examined, inspected, and tested, and which meet the minimum requirements set forth in Subparts H through M of this part, as applicable.

(b) The Bureau and the Institute will not issue certificates of approval for any respirator component or for any respirator subassembly.

(c) The Bureau and the Institute shall not issue an informal notification of approval. However, if the application for approval, submitted in accordance with § 11.11, states that the submitted respirator and component parts are only prototypes, the Bureau will examine, inspect, and test such respirator and component parts in accordance with the

provisions of this Part 11. If, upon completion of such examinations, inspections and tests, it is found that the prototype meets the minimum requirements set forth in this part, the Bureau and the Institute may inform the applicant, in writing, of the results of the examinations, inspections, and tests, and may require him to resubmit respirators and component parts made on regular production tooling, with no operations included which will not be incorporated in regular production processing, for further examination, inspection, and testing, prior to issuance of the certificate of approval.

(d) Applicants required to resubmit respirators and component parts made on regular production tooling, with no operation included which will not be incorporated in regular production processing, shall be charged fees in accordance with Subpart C of this part.

**§ 11.31 Certificates of approval; contents.**

(a) The certificate of approval shall contain a classification and a description of the respirator or combination of respirators for which it is issued, as provided in this part.

(b) The certificate of approval shall specifically set forth any restrictions or limitations on the respirator's use in hazardous atmospheres.

(c) Each certificate of approval shall be accompanied by the drawings and specifications (and lists thereof) submitted by the applicant in accordance with § 11.11. These drawings and specifications shall be incorporated by reference in the certificate of approval, and shall be maintained by the applicant. The drawings and specifications listed in each certificate of approval shall set forth in detail the design and construction requirements which shall be met by the applicant during commercial production of the respirator.

(d) Each certificate of approval shall be accompanied by a reproduction of the approval label design to be employed by the applicant with each approved respirator, as provided in § 11.33.

(e) No test data or specific laboratory findings will accompany any certificate of approval, however, the Bureau will release pertinent test data and specific findings upon written request by the applicant, or as required by statute or regulation.

(f) Each certificate of approval shall also contain the approved quality control plan as specified in § 11.42.

**§ 11.32 Notice of disapproval.**

(a) If, upon the completion of the examinations, inspections, and tests required to be conducted in accordance with the provisions of this part, it is found that the respirator does not meet the minimum requirements set forth in this part, the Bureau and the Institute shall issue a written notice of disapproval to the applicant.

(b) Each notice of disapproval shall be accompanied by all pertinent data or findings with respect to the defects of the

respirator for which approval was sought with a view to the possible correction of any such defects.

(c) The Bureau and the Institute shall not disclose, except to the applicant or as required by statute or regulation, any data, findings, or other information with respect to any respirator for which a notice of disapproval is issued.

**§ 11.33 Approval labels and markings; approval of contents; use.**

(a) Full-scale reproductions of approval labels and markings, and a sketch or description of the method of application and position on the harness, container, canister, cartridge, filter, or other component, together with instructions for the use and maintenance of the respirator shall be submitted to the Bureau and the Institute for approval.

(b) Approval labels shall bear the seals of the U.S. Bureau of Mines and the Department of Health, Education, and Welfare, the applicant's name and address, an approval number assigned by the Bureau, and, where appropriate, restrictions or limitations placed upon the use of the respirator by the Bureau and the Institute.

(c) The Bureau shall, where necessary, notify the applicant when additional labels, markings, or instructions will be required.

(d) Approval labels and markings shall only be used by the applicant to whom they were issued.

(e) Legible reproductions or abbreviated forms of the label approved by the Bureau and the Institute for use on each respirator shall be attached to or printed at the following locations:

| Respirator type                                                  | Label type   | Location                                                                             |
|------------------------------------------------------------------|--------------|--------------------------------------------------------------------------------------|
| Self-contained breathing apparatus.                              | Entire.....  | Harness assembly and canister (where applicable).                                    |
| Gas mask.....                                                    | Entire.....  | Mask container and canister.                                                         |
| Supplied-air respirator.                                         | Entire.....  | Respirator container or instruction card.                                            |
| Dust, fume, and mist respirator.                                 | Entire.....  | Respirator container and filter container.                                           |
|                                                                  | Abbreviated. | Filters.                                                                             |
| Chemical-cartridge respirator, including paint spray respirator. | Entire.....  | Respirator container, cartridge container, and filter containers (where applicable). |
|                                                                  | Abbreviated. | Cartridges and filters and filter containers.                                        |
| Pesticide respirator.                                            | Entire.....  | Respirator container, and cartridge and filter containers.                           |
|                                                                  | Abbreviated. | Cartridges and filters.                                                              |

(f) The use of any Bureau and Institute approval label obligates the applicant to whom it is issued to maintain or cause to be maintained the approved quality control sampling schedule and the acceptable quality level for each characteristic tested, and to assure that it is manufactured according to the drawings and specifications upon which the certificate of approval is based.

(g) Each respirator, respirator component, and respirator container shall, as

required by the Bureau and the Institute to assure quality control and proper use of the respirator, be labeled distinctly to show the name of the applicant, and the name and letters or numbers by which the respirator or respirator component is designated for trade purposes, and the lot number, serial number, or approximate date of manufacture.

**§ 11.34 Revocation of certificates of approval.**

The Bureau and the Institute reserve the right to jointly revoke, for cause, any certificate of approval issued pursuant to the provisions of this part. Such causes include, but are not limited to, misuse of approval labels and markings, misleading advertising, violations of section 109(e) of the Federal Coal Mine Health and Safety Act of 1969 (30 U.S.C. 819 (e)), and failure to maintain or cause to be maintained the quality control requirements of the certificate of approval.

**§ 11.35 Changes or modification of approved respirators; issuance of modification of certificate of approval.**

(a) Each applicant may, if he desires to change any feature of an approved respirator, request a modification of the original certificate of approval issued by the Bureau and the Institute for such respirator by filing an application for such modification in accordance with the provisions of this section.

(b) Applications shall be submitted as for an original certificate of approval, with a request for a modification of the existing certificate to cover any proposed change.

(c) The application shall be accompanied by appropriate drawings and specifications, and by a proposed quality control plan which meets the requirements of Subpart E of this part.

(d) The application for modification, together with the accompanying material, shall be examined by the Bureau to determine whether testing will be required.

(e) The Bureau shall inform the applicant of the fee required for any additional testing and the applicant will be charged for the actual cost of any examination, inspection, or test required, and such fees shall be submitted in accordance with the provisions of Subpart C of this part.

(f) If the proposed change or modification meets the requirements of this part, a formal certificate of modification will be issued, accompanied, where necessary, by a list of new and revised drawings and specifications covering the change(s) and reproductions of revised approval labels.

**§ 11.36 Delivery of changed or modified approved respirator.**

An approved respirator for which a formal certificate of modification has been issued shall be delivered, with proper markings and containers, by the applicant to the Bureau of Mines, Approval and Testing, 4800 Forbes Avenue, Pittsburgh, PA 15213, as soon as it is commercially produced.

**Subpart E—Quality Control****§ 11.40 Quality control plans, filing requirements.**

As a part of each application for approval or modification of approval submitted pursuant to this part, each applicant shall file with the Bureau and the Institute a proposed quality control plan which shall be designed to assure the quality of respiratory protection provided by the respirator for which approval is sought.

**§ 11.41 Quality control plans; contents.**

(a) Each quality control plan shall contain provisions for the management of quality, including: (1) Requirements for the production of quality data, and the use of quality control records; (2) control of engineering drawings, documentations, and changes; (3) control and calibration of measuring and test equipment; (4) control of purchased material to include incoming inspection; (5) lot identification, control of processes, manufacturing, fabrication, and assembly work conducted in the applicant's plant; (6) audit of final inspection of the completed product; and, (7) the organizational structure necessary to carry out these provisions.

(b) Each provision for incoming and final inspection in the quality control plan shall include a procedure for the selection of a sample of respirators and the components thereof for testing, in accordance with procedures set forth in Military Standard MIL-STD-105D, "Sampling Procedures and Tables for Inspection by Attributes," or Military Standard MIL-STD-414, "Sampling Procedures and Tables for Inspection by Variables for Percent Defective," or an approved equivalent sampling procedure, or an approved combination of sampling procedures. Incoming bulk raw material inspection or verification of specification, and in-process inspection shall be sufficient to ensure control of product quality through the manufacturing cycle.

(c) The sampling procedure shall include a list of the characteristics to be tested by the applicant or his agent.

(d) The characteristics listed in accordance with paragraph (c) of this section shall be classified according to the potential effect of such defect and grouped into the following classes:

(1) *Critical*. A defect that judgment and experience indicate is likely to result in a condition immediately hazardous to life or health for individuals using or depending upon the respirator;

(2) *Major A*. A defect, other than critical, that is likely to result in failure to the degree that the respirator does not provide any respiratory protection, or a defect that reduces protection and is not detectable by the user;

(3) *Major B*. A defect, other than Major A or critical, that is likely to result in reduced respiratory protection, and is detectable by the user; and

(4) *Minor*. A defect that is not likely to materially reduce the usability of the respirator for its intended purpose, or

a defect that is a departure from established standards and has little bearing on the effective use or operation of the respirator.

(e) The quality control inspection test method to be used by the applicant or his agent for each characteristic required to be tested shall be described in detail.

(f) Each item manufactured shall be 100 percent inspected for defects in all critical characteristics and all defective items shall be rejected.

(g) The Acceptable Quality Level (AQL) for each major or minor defect so classified by the applicant shall be:

- (1) *Major A*. 1.0 percent;
- (2) *Major B*. 2.5 percent; and
- (3) *Minor*. 4.0 percent.

(h) Except as provided in paragraph (i) of this section, inspection level II as described in MIL-STD-105D, or inspection level IV as described in MIL-STD-414, shall be used for major and minor characteristics and 100 percent inspection for critical characteristics.

(i) Subject to the approval of the Bureau and the Institute, where the quality control plan provisions for raw material, processes, manufacturing, and fabrication inspection are adequate to insure control of finished article quality, destructive testing of finished articles may be conducted at a lower level of inspection than that specified in paragraph (h) of this section.

**§ 11.42 Proposed quality control plans; approval by the Bureau and the Institute.**

(a) Each proposed quality control plan submitted in accordance with this subpart shall be reviewed by the Bureau and the Institute to determine its effectiveness in insuring the quality of respiratory protection provided by the respirator for which an approval is sought.

(b) If the Bureau and the Institute determine that the proposed quality control plan submitted by the applicant will not insure adequate quality control, the Bureau and the Institute shall require the applicant to modify the procedures and testing requirements of the plan prior to approval of the plan and issuance of any certificate of approval.

(c) Approved quality control plans shall constitute a part of and be incorporated into any certificate of approval issued by the Bureau and the Institute, and compliance with such plans by the applicant shall be a condition of approval.

**§ 11.43 Quality control records; review by the Bureau and the Institute; revocation of approval.**

(a) The applicant shall keep quality control inspection records sufficient to carry out the procedures required in MIL-STD-105D or MIL-STD-414, or an approved equivalent sampling procedure.

(b) The Bureau and the Institute reserve the right to have their representatives inspect the applicant's quality control test methods, equipment, and records, and to interview any employee or agent of the applicant in regard to quali-

ty control test methods, equipment, and records.

(c) The Bureau and the Institute reserve the right to jointly revoke, for cause, any certificate of approval where it is found that the applicant's quality control test methods, equipment, or records do not insure effective quality control over the respirator for which the approval was issued.

**Subpart F—Classification of Approved Respirators; Scope of Approval; Atmospheric Hazards; Service Time****§ 11.50 Types of respirators to be approved; scope of approval.**

Approvals shall be issued for the types of respirators which have been classified pursuant to this Subpart F, have been inspected, examined and tested by the Bureau in accordance with the provisions of Subparts G through M of this part, and have been found to provide respiratory protection for fixed periods of time against the hazards specified in such approval.

**§ 11.51 Entry and escape, or escape only; classification.**

Respirators described in Subparts H through M of this part shall be classified for use as follows:

(a) *Entry and escape*. Respirators designed and approved for use during entry into a hazardous atmosphere, and for escape from a hazardous atmosphere; or,

(b) *Escape only*. Respirators designed and approved for use only during escape from a hazardous atmosphere.

**§ 11.52 Respiratory hazards; classification.**

Respirators described in Subparts H through M of this part shall be classified as approved for use against any or all of the following respiratory hazards:

- (a) Oxygen deficiency;
- (b) Gases and vapors;
- (c) Particles, including dusts, fumes and mists; and
- (d) Pesticides.

**§ 11.53 Service time; classification.**

(a) Respirators described in Subparts H through M of this part shall be classified, where applicable, as approved for use during the following prescribed service times:

- (1) Four hours;
- (2) Three hours;
- (3) Two hours;
- (4) One hour;
- (5) Forty-five minutes;
- (6) Thirty minutes;
- (7) Fifteen minutes;
- (8) Ten minutes;
- (9) Five minutes;
- (10) Three minutes.

(b) Other service times may be prescribed by the Bureau and the Institute.

**Subpart G—General Construction and Performance Requirements****§ 11.60 Construction and performance requirements; general.**

(a) The Bureau and the Institute shall issue approvals for the types of respirators described in Subparts H through M

of this part which have met the minimum requirements set forth for such respirators in this Part 11.

(b) In addition to the types of respirators specified in Subparts H through M, the Bureau and the Institute shall issue approvals for other respiratory protective devices not specifically described in this Part 11 subject to such additional requirements as may be imposed in accordance with § 11.62(c).

**§ 11.61 General construction requirements.**

(a) Respirators will not be accepted by the Bureau for examination, inspection and testing unless they are designed on sound engineering and scientific principles, constructed of suitable materials and evidence good workmanship.

(b) Respirator components which come into contact with the wearer's skin shall be made of nonirritating materials.

(c) Components replaced during or after use shall be constructed of materials which will not be damaged by normal handling.

(d) Mouthpieces, hoods, helmets, and facepieces, except those employed in single-use respirators, shall be constructed of materials which will withstand repeated disinfection as recommended by the applicant in his instructions for use of the device.

(e) The components of each respirator approved by the Bureau and the Institute for use where permissibility is required shall meet the requirements for permissibility and intrinsic safety set forth in Part 18, Subchapter D of this chapter (Bureau of Mines Schedule 2G).

**§ 11.62 Component parts; minimum requirements.**

(a) The component parts of each respirator shall be:

(1) Designed, constructed, and fitted to insure against creation of any hazard to the wearer;

(2) Assembled to permit easy access for inspection and repair of functional parts; and

(3) Assembled to permit easy access to parts which require periodic cleaning and disinfecting.

(b) Replacement parts shall be designed and constructed to permit easy installation and to maintain the effectiveness of the respirator.

**§ 11.63 Test requirements; general.**

(a) Each respirator and respirator component shall when tested by the applicant and by the Bureau, meet the applicable requirements set forth in Subparts H through M of this part.

(b) Where a combination respirator is assembled from two or more types of respirators, as described in this part, each of the individual respirator types which have been combined shall, as applicable, meet the minimum requirements for such respirators set forth in Subparts H through M of this part, and such combination respirators, except as specified in § 11.70(b) (2), will be classified by the type of respirator in the combination which provides the least protection to the user.

(c) In addition to the minimum requirements set forth in Subparts H through M of this part, the Bureau and the Institute reserve the right to require, as a further condition of approval, any additional requirements deemed necessary to establish the quality, effectiveness, and safety of any respirator used as protection against hazardous atmospheres.

(d) Where it is determined after receipt of an application that additional requirements will be required for approval, the Bureau will notify the applicant in writing of these additional requirements, and necessary examinations, inspections, or tests, stating generally the reasons for such requirements, examinations, inspections, or tests.

**§ 11.64 Pretesting by applicant; approval of test methods by the Bureau.**

(a) Prior to making or filing any application for approval or modification of approval, the applicant shall conduct, or cause to be conducted, examinations, inspections, and tests of respirator performance which are equal to or exceed the severity of those prescribed in this part.

(b) With the application, the applicant shall provide a statement to the Bureau showing the types and results of the examinations, inspections, and tests required under paragraph (a) of this section and state that the respirator meets the minimum requirements of Subparts H through M of this part, as applicable. Complete examination, inspection, and test data shall be retained on file by the applicant and be submitted, upon request, to the Bureau.

(c) The Bureau may, upon written request by the applicant, provide drawings and descriptions of its test equipment and otherwise assist the applicant in establishing a test laboratory or securing the services of a testing agency.

(d) The Bureau will not issue an approval to the applicant until it has validated the applicant's test results.

**§ 11.65 Conduct of examinations, inspections, and tests by the Bureau and the Institute; assistance by applicant; observers; recorded data; public demonstrations.**

(a) All examinations, inspections, and tests conducted pursuant to Subparts H through M of this part will be under the sole direction and control of the Bureau and the Institute.

(b) The Bureau and the Institute may, as a condition of approval, require the assistance of the applicant or agents of the applicant during the assembly, disassembly, or preparation of any respirator or respirator component prior to testing or in the operation of such equipment during testing.

(c) Only Bureau and Institute personnel, persons assisting the Bureau pursuant to paragraph (b) of this section, and such other persons as are requested by the Bureau, the Institute, or the applicant to be observers, shall be present during any examination, inspection, or test conducted prior to the issuance of an ap-

proval by the Bureau and the Institute for the equipment under consideration.

(d) The Bureau and the Institute shall hold as confidential any analyses, drawings, specifications, or materials submitted by the applicant and shall not disclose any principles or patentable features of such equipment, except as required by statute or regulation.

(e) As a condition of each approval issued for any respirator, the Bureau and the Institute reserve the right, following the issuance of such approval, to conduct such public tests and demonstrations of the approved respiratory equipment as is deemed appropriate.

**§ 11.66 Withdrawal of applications; refund of fees.**

(a) Any applicant may, upon a written request submitted to the Bureau or the Institute, withdraw any application for approval of any respirator.

(b) Upon receipt of a written request for the withdrawal of an application, the Bureau shall determine the total man-days expended and the amount due for services already performed during the course of any examinations, inspections, or tests conducted pursuant to such application. The total amount due shall be determined in accordance with the provisions of § 11.22 and assessed against the fees submitted by the applicant. If the total amount assessed is less than the fees submitted, the Bureau shall refund the balance together with a statement of the charges made for services rendered.

**Subpart H—Self-Contained Breathing Apparatus**

**§ 11.70 Self-contained breathing apparatus; description.**

(a) Self-contained breathing apparatus, including all completely assembled, portable, self-contained devices designed for use as respiratory protection during entry into and escape from or escape only from hazardous atmospheres, are described as follows:

(1) *Closed-circuit apparatus.* An apparatus of the type in which the exhalation is rebreathed by the wearer after the carbon dioxide has been effectively removed and a suitable oxygen concentration restored from sources composed of:

- (i) Compressed oxygen; or
- (ii) Chemical oxygen; or
- (iii) Liquid-oxygen.

(2) *Open-circuit apparatus.* An apparatus of the following types from which exhalation is vented to the atmosphere and not rebreathed:

(i) *Demand-type apparatus.* An apparatus in which the pressure inside the facepiece in relation to the immediate environment is positive during exhalation and negative during inhalation.

(ii) *Pressure-demand-type apparatus.* An apparatus in which the pressure inside the facepiece in relation to the immediate environment is positive during both inhalation and exhalation.

(b) The following respirators may be classified as designed and approved for

use during emergency entry into a hazardous atmosphere: A combination respirator which includes a self-contained breathing apparatus and a Type "C" or Type "CE" supplied air respirator, where (1) the self-contained breathing apparatus is classified for 3-, 5-, or 10-minute service time and the air line supply is used during entry, or (2) the self-contained breathing apparatus is classified for 15 minutes or longer service time and not more than 20 percent of the rated capacity of the air supply is used during entry.

(c) Self-contained breathing apparatus classified for less than 1 hour service time will not be approved for use during underground mine rescue and recovery operations except as auxiliary equipment.

(d) Self-contained breathing apparatus classified for less than 30 minutes' service time will not be approved for use as auxiliary equipment during underground mine rescue and recovery operations.

**§ 11.71 Self-contained breathing apparatus; required components.**

(a) Each self-contained breathing apparatus described in § 11.70 shall, where its design requires, contain the following component parts:

- (1) Facepiece or mouthpiece, and noseclip;
- (2) Respirable breathing gas container;
- (3) Supply of respirable breathing gas;
- (4) Gas pressure or liquid level gages;
- (5) Timer;
- (6) Remaining service life indicator or warning device;
- (7) Hand-operated valves;
- (8) Breathing bag;
- (9) Safety relief valve or safety relief system; and
- (10) Harness.

(b) The components of each self-contained breathing apparatus shall meet the minimum construction requirements set forth in Subpart G of this part.

**§ 11.72 Breathing tubes; minimum requirements.**

(a) Flexible breathing tubes used in conjunction with breathing apparatus shall be designed and constructed to prevent:

- (1) Restriction of free head movement;
- (2) Disturbance of the fit of facepieces and mouthpieces;
- (3) Interference with the wearer's activities; and,
- (4) Shutoff of airflow due to kinking, or from chin or arm pressure.

**§ 11.73 Harnesses; installation and construction; minimum requirements.**

(a) Each apparatus shall, where necessary, be equipped with a suitable harness designed and constructed to hold the components of the apparatus in position against the wearer's body.

(b) Harnesses shall be designed and constructed to permit easy removal and replacement of apparatus parts, and,

where applicable, provide for holding a full facepiece in the ready position when not in use.

**§ 11.74 Apparatus containers; minimum requirements.**

(a) Apparatus may be equipped with a substantial, durable container bearing markings which show the applicant's name, the type and commercial designation of the respirator it contains, and all appropriate approval labels.

(b) Containers supplied by the applicant for carrying or storing self-contained breathing apparatus will be inspected, examined, and tested as components of the respirator for which approval is sought.

(c) Containers for self-contained breathing apparatus shall be designed and constructed to permit easy removal of the apparatus.

**§ 11.75 Half-mask facepieces, full facepieces, mouthpieces; fit; minimum requirements.**

(a) Half-mask facepieces and full facepieces shall be designed and constructed to fit persons with various facial shapes and sizes, either (1) by providing more than one facepiece size, or (2) by providing one facepiece size which will fit varying facial shapes and sizes.

(b) Full facepieces shall provide for the optional use of corrective spectacles or lenses which shall not reduce the respiratory protective qualities of the apparatus.

(c) Apparatus with mouthpieces shall be equipped with noseclips which are securely attached to the mouthpiece or apparatus and provide an airtight seal.

(d) Facepieces shall be designed to prevent eyepiece, spectacle, and lens fogging.

**§ 11.76 Facepieces; eyepieces; minimum requirements.**

(a) Facepieces shall be designed and constructed to provide adequate vision which is not distorted by the eyepiece.

(b) All eyepieces shall be designed and constructed to meet the impact and penetration requirements specified in Federal Specification, Mask, Air Line, and Respirator, Air Filtering, Industrial, GGG-M-125d, October 11, 1965. This Federal Specification is available from the Government Printing Office or the General Services Administration.

**§ 11.77 Inhalation and exhalation valves; minimum requirements.**

(a) Inhalation and exhalation valves shall be provided where necessary and protected against damage and distortion.

(b) Exhalation valves shall be:

- (1) Protected against external influence, and
- (2) Designed and constructed to prevent inward leakage of contaminated air.

**§ 11.78 Head harnesses; minimum requirements.**

(a) Facepieces shall be equipped with adjustable and replaceable head harnesses designed and constructed to pro-

vide adequate tension during suspension and an even distribution of pressure over the entire area in contact with the face.

(b) Mouthpieces shall be equipment where applicable, with adjustable and replaceable harnesses designed and constructed to hold the mouthpiece in place.

**§ 11.79 Breathing gas; minimum requirements.**

(a) Breathing gas used to supply apparatus shall be respirable and contain no less than 19.5 (dry atmosphere) volume percent of oxygen.

(b) Oxygen, including liquid oxygen, shall meet the minimum requirements for medical or breathing oxygen set forth in the U.S. Pharmacopeia.

(c) Compressed, gaseous breathing air shall meet the applicable minimum grade requirements for Type I gaseous air set forth in the Compressed Gas Association Commodity Specification for Air, G-7.1 (Grade D or higher quality).

(d) Compressed, liquefied breathing air shall meet the applicable minimum grade requirements for Type II liquid air set forth in the Compressed Gas Association Commodity Specification for Air, G-7.1 (Grade B or higher quality).

**§ 11.79-1 Interchangeability of oxygen and air prohibited.**

Approvals shall not be issued by the Bureau and the Institute for any apparatus, combination of respirator assemblies, or any apparatus or respirator component which is designed or constructed to permit the interchangeable use of oxygen and air.

**§ 11.80 Compressed breathing gas and liquefied breathing gas containers; minimum requirements.**

(a) Compressed breathing gas and liquefied breathing gas containers shall meet the minimum requirements of the Department of Transportation for Interstate shipment of such containers when fully charged.

(b) Such containers shall be permanently and legibly marked to identify their contents, e.g., compressed breathing air, compressed breathing oxygen, liquefied breathing air, or liquefied breathing oxygen.

(c) Containers normally removed from apparatus for refilling shall be equipped with a dial indicating gage which shows the pressure in the container.

(d) Compressed breathing gas contained valves or a separate charging system or adapter provided with each apparatus shall be equipped with outlet threads specified for the service by the American National Standard for Compressed Gas Cylinder Valve Outlet and Inlet Connections, B57.1 (1965), obtainable from American National Standards Institute, Inc., 1430 Broadway, New York, NY 10018.

**§ 11.81 Gas pressure gages; minimum requirements.**

(a) Gas pressure gages employed on compressed breathing gas containers shall be calibrated in pounds per square inch.

(b) Liquid-level gages shall be calibrated in fractions of total container capacity, or in units of liquid volume.

(c) Gas pressure gages other than those specified in paragraphs (a) and (b) of this section shall be calibrated in:

(1) Pounds per square inch, or  
(2) In fractions of total container capacity, or

(3) Both in pounds per square inch and in fractions of total container capacity.

(d) (1) Dial-indicating gages shall be reliable to within  $\pm 5$  percent of full scale when tested both up and down the scale at each of 5 equal intervals.

(2) The full scale graduation of dial-indicating gages shall not exceed 150 percent of the maximum rated cylinder pressures specified for the container in applicable Department of Transportation specifications or permits.

(e) (1) Stem-type gages shall be readable by sight and by touch and shall have a stem travel distance of not less than one-fourth inch between each graduation.

(2) A minimum of five graduations shall be engraved on the stem of each gage and these graduations shall include readings for empty, one-quarter, one-half, three-quarters, and full.

(3) Stem gage readings shall not vary from true readings by more than one-sixteenth inch per inch of stem travel.

(f) The loss of gas through a broken gage or severed gage connection shall not exceed 70 liters per minute when the cylinder pressure is 6,900 kN/m<sup>2</sup> (1,000 pounds per square inch gage) or when the liquid level is at one-half.

(g) Where gages are connected to the apparatus through a gage line, the gage and line shall be capable of being isolated from the apparatus except where the failure of the gage or line would not impair the performance or service life of the apparatus.

(h) Oxygen pressure gages shall have the words, "Oxygen" and "Use No Oil," marked prominently on the gage.

(i) (1) Apparatus using compressed breathing gas, except apparatus classified for escape only, shall be equipped with gages visible to the wearer which indicate the remaining gas content in the container.

(2) Apparatus using liquefied breathing gas, except apparatus classified for escape only, shall be equipped with gages visible to the wearer which indicate the remaining liquid content in the container; however, where the liquid content cannot be rapidly vented, and the service time of the device begins immediately after filling, a timer shall be provided in place of a visible gage.

§ 11.82 Timers; elapsed time indicators; remaining service life indicators; minimum requirements.

(a) Elapsed time indicators shall be provided for apparatus with a chemical oxygen source, except:

(1) Apparatus used for escape only; or,

(2) Liquefied breathing gas apparatus equipped with gages visible to the wearer

which indicate the remaining liquid content in the container.

(b) The timer or other indicator shall be accurately calibrated in minutes of remaining service life.

(c) Timers shall be readable by sight and by touch during use by the wearer.

(d) Timers shall be equipped with automatically preset alarms which will warn the wearer for a period of 7 seconds or more after the preset time has elapsed.

(e) Remaining service-life indicators or warning devices shall be provided in addition to a pressure gage on compressed gas self-contained breathing apparatus, except apparatus used for escape only, and shall operate automatically without preadjustment by the wearer.

(f) Each remaining service-life indicator or warning device shall give an alarm when the remaining service life of the apparatus is reduced within a range of 20 to 25 percent of its rated service time.

§ 11.83 Hand-operated valves; minimum requirements.

(a) Hand-operated valves shall be designed and constructed to prevent removal of the stem from the valve body during normal usage to insure against a sudden release of the full pressure of the container when the valve is opened.

(b) Valves shall be designed or positioned to prevent accidental opening and closing, and damage from external forces.

(c) Valves operated during use of the apparatus shall be installed in locations where they can be readily adjusted by the wearer.

(d) Main-line valves, designed and constructed to conserve gas in the event of a regulator or demand valve failure, shall be provided in addition to gas container valves, except when such failure will not affect performance.

(e) Hand-operated bypass systems designed and constructed to permit the wearer to breathe and to conserve his gas supply in the event of a regulator or demand valve failure, shall be provided where necessary.

(f) Valves installed on apparatus shall be clearly distinguishable from one another by sight and touch.

(g) The bypass system valve control shall be colored red.

(h) A main-line or bypass valve or system will not be required on apparatus for escape only.

(i) Safety relief valves or systems, designed and constructed to release excess pressure in the breathing circuit, shall be provided on closed-circuit apparatus, and shall meet the following requirements:

(1) The relief valve or system shall operate automatically when the pressure in the breathing circuit on the inhalation side of the breathing bag reaches 13 mm. (one-half inch) water-column height of pressure above the minimum pressure required to fill the breathing bag, within the breathing resistance requirements for the apparatus.

(2) The relief valve or system shall be designed to prevent external atmospheres from entering the breathing circuit.

(3) The relief valve or system shall be designed to permit manual overriding for test purposes and in the event of a failure in the valve or system.

§ 11.84 Breathing bags; minimum requirements.

(a) Breathing bags shall have sufficient volume to prevent gas waste during exhalation and to provide an adequate reserve for inhalation.

(b) Breathing bags shall be constructed of materials which are flexible and resistant to gasoline vapors.

(c) Breathing bags shall be installed in a location which will protect them from damage or collapse by external forces, except on apparatus classified for escape only.

§ 11.85 Self-contained breathing apparatus; performance requirements; general.

Self-contained breathing apparatus and the individual components of each such device shall as applicable meet the requirements specified in §§ 11.85-1 through 11.85-19.

§ 11.85-1 Component parts exposed to oxygen pressures; minimum requirements.

Each applicant shall certify that the materials employed in the construction of component parts exposed to oxygen pressures above atmospheric pressure are safe and compatible for their intended use.

§ 11.85-2 Compressed gas filters; minimum requirements.

All self-contained breathing apparatus using compressed gas shall have a filter downstream of the gas source to effectively remove particles from the gas stream.

§ 11.85-3 Breathing bag test.

(a) Breathing bags will be tested in an air atmosphere saturated with gasoline vapor at room temperature (24°-30° C./75°-85° F.) for a continuous period of twice the rated time of the apparatus (except for apparatus for escape only where the test period shall be the rated time of the apparatus).

(b) The bag will be operated during this test by a breathing machine with 24 respirations per minute and a minute-volume of 40 liters.

(c) A breathing machine cam with a work rate of 622 kg.-m./min. will be used.<sup>1</sup>

(d) The air within the bag(s) shall not contain more than 100 parts per million of gasoline vapor at the end of the test.

<sup>1</sup> Silverman, L., G. Lee, T. Plotkin, L. Amory, and A. R. Yancey, Fundamental Factors in Design of Protective Equipment, O.S.R.D. Report No. 5732, Issued Apr. 1, 1945. The dimensions of the breathing machine cam are available from the Bureau upon request.

**§ 11.85-4 Weight requirement.**

(a) The completely assembled and fully charged apparatus shall not weigh more than 16 kg. (35 pounds); however, where the weight decreases by more than 25 percent of its initial charge weight during its rated service life, the maximum allowable weight of a completely assembled and fully charged apparatus shall be 18 kg. (40 pounds).

(b) Where an apparatus employs equipment which contributes materially to the wearer's comfort, e.g., a cooling system, the completely assembled and fully charged apparatus shall not weigh more than 18 kg. (40 pounds) regardless of the decrease in weight during use.

**§ 11.85-5 Breathing resistance test; inhalation.**

(a) Resistance to inhalation airflow will be measured in the facepiece or mouthpiece while the apparatus is operated by a breathing machine as described in § 11.85-3.

(b) The inhalation resistance of open-circuit apparatus shall not exceed 32 mm. (1.25 inch) water-column height (at a flow rate of 120 liters per minute).

(c) The inhalation resistance of closed-circuit apparatus shall not exceed the difference between exhalation resistance (§ 11.85-6(e)) and 10 cm. (4 inches) water-column height.

**§ 11.85-6 Breathing resistance test; exhalation.**

(a) Resistance to exhalation airflow will be measured in the facepiece or mouthpiece of open-circuit apparatus with air flowing at a continuous rate of 85 liters per minute.

(b) The exhalation resistance of demand apparatus shall not exceed 25 mm. (1 inch) water-column height.

(c) The exhalation resistance of pressure-demand apparatus shall not exceed the static pressure in the facepiece by more than 51 mm. (2 inches) water-column height.

(d) The static pressure (at zero flow) in the facepiece shall not exceed 38 mm. (1.5 inches) water-column height.

(e) Resistance to exhalation airflow will be measured in the facepiece or mouthpiece of closed-circuit apparatus with a breathing machine as described in § 11.85-3, and the exhalation resistance shall not exceed 51 mm. (2 inches) water-column height.

**§ 11.85-7 Exhalation valve leakage test.**

(a) Dry exhalation valves and valve seats will be subjected to a suction of 25 mm. (1 inch) water-column height while in a normal operating position.

(b) Leakage between the valve and the valve seat shall not exceed 30 milliliters per minute.

**§ 11.85-8 Gas flow test; open-circuit apparatus.**

(a) A static-flow test will be performed on all open-circuit apparatus.

(b) The flow from the apparatus shall be greater than 200 liters per minute when the pressure in the facepiece of

demand-apparatus is lowered by 51 mm. (2 inches) water-column height when full container pressure is applied.

(c) Where pressure demand apparatus are tested, the flow will be measured at zero gage pressure in the facepiece.

(d) Where apparatus with compressed-breathing-gas containers are tested, the flow test shall also be made with 3,450 kN/m<sup>2</sup> (500 p.s.i.g.) container pressure applied.

**§ 11.85-9 Gas flow test; closed-circuit apparatus.**

(a) Where oxygen is supplied by a constant-flow device only, the rate of flow shall be at least 3 liters per minute for the entire rated service time of the apparatus.

(b) Where constant flow is used in conjunction with demand flow, the constant flow shall be greater than 1.5 liters per minute for the entire rated service time.

(c) All demand-flow devices shall provide at least 30 liters of oxygen per minute when in the fully open position.

**§ 11.85-10 Service time test; open-circuit apparatus.**

(a) Service time will be measured with a breathing machine as described in § 11.85-3.

(b) The open-circuit apparatus will be classified according to the length of time it supplies air or oxygen to the breathing machine.

(c) The service time obtained on this test will be used to classify the open-circuit apparatus in accordance with § 11.53.

**§ 11.85-11 Service time test; closed-circuit apparatus.**

(a) The closed-circuit apparatus will be classified according to the length of time it supplies adequate breathing gas to the wearer during man test No. 4 described in Table 4.

(b) The service time obtained on man test No. 4 will be used to classify the closed-circuit apparatus in accordance with § 11.53.

**§ 11.85-12 Test for carbon dioxide in inspired gas; open- and closed-circuit apparatus; maximum allowable limits.**

(a) Open-circuit apparatus:

(1) The concentration of carbon dioxide in inspired gas in open-circuit apparatus will be measured at the mouth while the apparatus mounted on a dummy head is operated by a breathing machine.<sup>2</sup>

(2) The breathing rate will be 14.5 respirations per minute with a minute-volume of 10.5 liters.

(3) A sedentary breathing machine can will be used.

(4) The apparatus will be tested at a temperature of 27°±2° C. (80°±5° F.).

<sup>2</sup> Kloos, E. J., and J. Lamonica, A Machine-Test Method for Measuring Carbon Dioxide in the Inspired Air of Self-Contained Breathing Apparatus. Bureau of Mines Report of Investigations 6865, 1966, 11 pp.

(5) A concentration of 5 percent carbon dioxide in air will be exhaled into the facepiece.

(b) Closed-circuit apparatus:

(1) The concentration of carbon dioxide in inspired gas in closed-circuit apparatus will be measured at the mouth while the parts of the apparatus contributing to dead-air space are mounted on a dummy head and operated by the breathing machine as in paragraphs (a) (1) through (5) of this section.

(c) During the testing required by paragraphs (a) and (b) of this section, the concentration of carbon dioxide in inspired gas at the mouth will be continuously recorded, and the maximum average concentration during the inhalation portion of the breathing cycle shall not exceed the following limits:

| Where the service time is: | Maximum allowable average concentration of carbon dioxide in inspired air, percent by volume |
|----------------------------|----------------------------------------------------------------------------------------------|
| Not more than 30 minutes   | 2.5                                                                                          |
| 1 hour                     | 2.0                                                                                          |
| 2 hours                    | 1.5                                                                                          |
| 3 hours                    | 1.0                                                                                          |
| 4 hours                    | 1.0                                                                                          |

(d) In addition to the tests requirements for closed-circuit apparatus set forth in paragraph (b) of this section, gas samples will be taken during the course of the man tests described in Tables 1, 2, 3, and 4. These gas samples will be taken from the closed-circuit apparatus at a point downstream of the carbon dioxide sorbent, and they shall not contain more than 0.5 percent carbon dioxide at any time.

**§ 11.85-13 Tests during low temperature operation.**

(a) The applicant shall specify the minimum temperature for safe operation and two persons will perform the tests described in paragraphs (c) and (d) of this section, wearing the apparatus according to applicant's directions. At the specified temperature, the apparatus shall meet all the requirements described in paragraph (e) of this section.

(b) The apparatus will be precooled at the specified minimum temperature for 4 hours.

(c) The apparatus will be worn in the low temperature chamber for 30 minutes, or for the service time of the apparatus, whichever is less.

(d) During the test period, alternate 1-minute periods of exercise and rest will be required with the exercise periods consisting of stepping onto and off a box 21.5 cm. (8½ inches) high at a rate of 30 cycles per minute.

(e) (1) The apparatus shall function satisfactorily at the specified minimum temperature on duplicate tests.

(2) The wearer shall have sufficient unobscured vision to perform the work.

(3) The wearer shall not experience undue discomfort because of airflow restriction or other physical or chemical changes in the operation of the apparatus.

(f) Auxiliary low-temperature parts which are commercially available to the user may be used on the apparatus to meet the requirements described in paragraph (e) of this section.

**§ 11.85-14 Man tests; testing conditions; general requirements.**

(a) The man tests described in Tables 1, 2, 3, and 4 represent the workload performed in the mining, mineral, or allied industries by a person wearing the apparatus tested.

(b) The apparatus tested will be worn by Bureau personnel trained in the use of self-contained breathing apparatus, and the wearer will, before participating in these tests, pass a physical examination conducted by a qualified physician.

(c) All man tests will be conducted by the Bureau.

(d) The apparatus will be examined before each man test to ensure that it is in proper working order.

(e) Breathing resistance will be measured within the facepiece or mouthpiece and the wearer's pulse and respiration rate will be recorded during each 2 minute sample period prescribed in tests 1, 2, 3, and 4.

(f) Man tests 1, 2, 3, 4, 5, and 6 will be conducted in duplicate.

(g) If man tests are not completed through no fault of the apparatus, the test will be repeated.

**§ 11.85-15 Man tests 1, 2, 3, and 4; requirements.**

(a) Man tests 1, 2, 3, and 4, set forth in Tables 1, 2, 3, and 4 respectively, prescribe the duration and sequence of specific activities. These tests will be conducted to:

(1) Familiarize the wearer with the apparatus during use;

(2) Provide for a gradual increase in activity;

(3) Evaluate the apparatus under different types of work and physical orientation; and

(4) Provide information on the operating and breathing characteristics of the apparatus during actual use.

**§ 11.85-16 Man test 5; requirements.**

(a) Test 5 will be conducted to determine the maximum length of time the apparatus will supply the respiratory needs of the wearer while he is sitting at rest.

(b) The wearer will manipulate the devices controlling the supply of breathing gas to the advantage of the apparatus.

(c) Samples of inspiration from within the apparatus facepiece or mouthpiece shall be taken once every 15 minutes, and shall meet the minimum requirement for oxygen specified in § 11.79(a) of this part, and the maximum allowable average concentration of carbon dioxide specified in § 11.85-12(c).

(d) One sample of inspiration will be taken in the case of 3-, 5-, and 10-minute apparatus.

**§ 11.85-17 Man test 6; requirements.**

(a) Man test 6 will be conducted with respect to liquefied breathing gas apparatus only.

(b) This test will be conducted to evaluate operation of the apparatus in other than vertical positions.

(c) The wearer will lie face downward for one-fourth the service life of the apparatus with a full charge of liquefied breathing gas, and then a one-quarter full charge of liquefied breathing gas.

(d) The test will be repeated with the wearer lying on each side and on his back.

(e) The oxygen content of the gas supplied to the wearer by the apparatus will be continuously measured.

**§ 11.85-18 Man tests; performance requirements.**

(a) The apparatus shall satisfy the respiratory requirements of the wearer for the classified service time.

(b) Fogging of the eyepiece shall not obscure the wearer's vision, and the wearer shall not experience undue discomfort because of fit or other characteristics of the apparatus.

(c) When the ambient temperature during testing is  $24^{\circ} \pm 6^{\circ}$  C. ( $75^{\circ} \pm 10^{\circ}$  F.), the maximum temperature of inspired air recorded during man tests shall not exceed the following, after correction for deviation from  $24^{\circ}$  C. ( $75^{\circ}$  F.):

| Where service life of apparatus is—          | Where percent relative humidity of inspired air is— | Maximum permissible temperature of inspired air shall not exceed— |               |
|----------------------------------------------|-----------------------------------------------------|-------------------------------------------------------------------|---------------|
|                                              |                                                     | $^{\circ}$ F.                                                     | $^{\circ}$ C. |
| $\frac{1}{4}$ hour or less.....              | 0-100                                               | 135                                                               | 57            |
| $\frac{1}{2}$ hour to $\frac{3}{4}$ hour.... | 0-50                                                | 125                                                               | 52            |
|                                              | 50-100                                              | 110                                                               | 43            |
| 1 to 2 hours.....                            | 0-50                                                | 115                                                               | 46            |
|                                              | 50-100                                              | 105                                                               | 41            |
| 3 hours.....                                 | 0-50                                                | 110                                                               | 43            |
|                                              | 50-100                                              | 100                                                               | 38            |
| 4 hours.....                                 | 0-50                                                | 105                                                               | 41            |
|                                              | 50-100                                              | 95                                                                | 35            |

<sup>1</sup> Where percent relative humidity is 50-100 and apparatus is designed for escape only, these maximum permissible temperatures will be increased by  $5^{\circ}$  C. ( $10^{\circ}$  F.).

**§ 11.85-19 Gas tightness test; minimum requirements.**

(a) Each apparatus will be tested for tightness by persons wearing it in an atmosphere of 1,000 p.p.m. isoamyl acetate.

(b) Six persons will each wear the apparatus in the test concentrations specified in paragraph (a) of this section for 2 minutes and none shall detect the odor or taste of the test vapor.

TABLE 1.—DURATION AND SEQUENCE OF SPECIFIC ACTIVITIES FOR TEST 1, IN MINUTES  
(30 CFR Part 11, Subpart H, § 11.85, et seq.)

| Activity                                 | Service time— |           |            |            |            |            |        |                                                      |
|------------------------------------------|---------------|-----------|------------|------------|------------|------------|--------|------------------------------------------------------|
|                                          | 3 minutes     | 5 minutes | 10 minutes | 15 minutes | 30 minutes | 45 minutes | 1 hour | 2, 3, and 4 hours                                    |
| Sampling and readings.....               |               |           |            |            | 2          | 2          | 2      | 2 Perform 1 hour test 2, 3, or 4 times respectively. |
| Walks at 4.8 km. (3 miles) per hour..... |               | 3         | 5          | 3          | 4          | 8          | 12     | 18                                                   |
| Sampling and readings.....               |               |           |            | 2          | 2          | 2          | 2      | 2                                                    |
| Walks at 4.8 km. (3 miles) per hour..... |               |           |            | 3          | 5          | 8          | 12     | 18                                                   |
| Sampling and readings.....               |               |           |            | 2          | 2          | 2          | 2      | 2                                                    |
| Walks at 4.8 km. (3 miles) per hour..... |               |           |            |            | 6          | 13         | 18     | 18                                                   |
| Sampling and readings.....               |               |           |            |            | 2          | 2          | 2      | 2                                                    |

## RULES AND REGULATIONS

TABLE 2.—DURATION AND SEQUENCE OF SPECIFIC ACTIVITIES FOR TEST 2, IN MINUTES  
(30 CFR Part 11, Subpart H, § 11.85, et seq.)

| Activity                                                                      | Service Time— |           |                      |                      |                       |                       |                        |
|-------------------------------------------------------------------------------|---------------|-----------|----------------------|----------------------|-----------------------|-----------------------|------------------------|
|                                                                               | 3 minutes     | 5 minutes | 10 minutes           | 15 minutes           | 30 minutes            | 45 minutes            | 1 hour                 |
| Sampling and readings.....                                                    |               |           |                      | 2.....               | 2.....                | 2.....                | 2.....                 |
| Walks at 4.8 km. (3 miles) per hour.....                                      |               |           | 1.....               | 1.....               | 3.....                | 4.....                | 6.....                 |
| Carries 23 kg. (50 pound) weight over overcast.....                           |               |           | 1 time in 2 minutes. | 1 time in 2 minutes. | 2 times in 4 minutes. | 3 times in 6 minutes. | 4 times in 8 minutes.  |
| Walks at 4.8 km. (3 miles) per hour.....                                      |               |           | 1.....               | 1.....               | 3.....                | 3.....                | 3.....                 |
| Climbs vertical treadmill <sup>1</sup> (or equivalent).....                   | 1.....        | 1.....    | 1.....               | 1.....               | 1.....                | 1.....                | 1.....                 |
| Walks at 4.8 km. (3 miles) per hour.....                                      |               | 1.....    | 1.....               |                      |                       | 2.....                | 3.....                 |
| Climbs vertical treadmill (or equivalent).....                                |               | 1.....    |                      |                      |                       | 1.....                | 1.....                 |
| Sampling and readings.....                                                    |               |           |                      | 2.....               | 2.....                | 2.....                | 2.....                 |
| Walks at 4.8 km. (3 miles) per hour.....                                      |               |           |                      | 2.....               | 2.....                | 3.....                | 6.....                 |
| Climbs vertical treadmill (or equivalent).....                                |               |           |                      | 1.....               | 1.....                | 1.....                | 1.....                 |
| Carries 23 kg. (50 pound) weight over overcast.....                           |               |           |                      | 1 time in 2 minutes. | 3 times in 6 minutes. | 4 times in 8 minutes. | 5 times in 10 minutes. |
| Sampling and readings.....                                                    |               |           | 2.....               |                      |                       | 2.....                | 2.....                 |
| Walks at 4.8 km. (3 miles) per hour.....                                      |               |           |                      | 1.....               | 3.....                | 3.....                | 3.....                 |
| Climbs vertical treadmill (or equivalent).....                                |               |           | 1.....               | 1.....               | 1.....                | 1.....                | 1.....                 |
| Walks at 4.8 km. (3 miles) per hour.....                                      |               |           | 2.....               |                      |                       | 2.....                | 3.....                 |
| Climbs vertical treadmill (or equivalent).....                                |               |           |                      |                      |                       | 1.....                | 1.....                 |
| Carries 20 kg. (45 pound) weight and walks at 4.8 km. (3 miles) per hour..... | 1.....        | 2.....    |                      |                      |                       |                       | 2.....                 |
| Sampling and readings.....                                                    |               |           |                      | 2.....               | 2.....                | 2.....                | 2.....                 |

<sup>1</sup> Total test time for Test 2 for 2-hour, 3-hour, and 4-hour apparatus is 2 hours.<sup>2</sup> Treadmill shall be inclined 15° from vertical and operated at a speed of 1 foot per second.TABLE 3.—DURATION AND SEQUENCE OF SPECIFIC ACTIVITIES FOR TEST 3, IN MINUTES  
(30 CFR Part 11, Subpart H, § 11.85, et seq.)

| Activity                                      | Service time— |                       |                        |                        |                        |                        |                        |
|-----------------------------------------------|---------------|-----------------------|------------------------|------------------------|------------------------|------------------------|------------------------|
|                                               | 3 minutes     | 5 minutes             | 10 minutes             | 15 minutes             | 30 minutes             | 45 minutes             | 1 hour                 |
| Sampling and readings.....                    |               |                       |                        | 2.....                 | 2.....                 | 2.....                 | 2.....                 |
| Walks at 4.8 km. (3 miles) per hour.....      |               |                       | 1.....                 | 1.....                 | 2.....                 | 2.....                 | 3.....                 |
| Runs at 9.7 km. (6 miles) per hour.....       | 1.....        | 1.....                | 1.....                 | 1.....                 | 1.....                 | 1.....                 | 1.....                 |
| Pulls 20 kg. (45 pound) weight to 5 feet..... |               | 15 times in 1 minute. |                        | 30 times in 2 minutes. | 30 times in 2 minutes. | 30 times in 2 minutes. | 60 times in 6 minutes. |
| Lies on side.....                             | ½.....        | 1.....                | 1.....                 | 2.....                 | 3.....                 | 4.....                 | 5.....                 |
| Lies on back.....                             | ½.....        | 1.....                | 1.....                 | 2.....                 | 2.....                 | 3.....                 | 3.....                 |
| Crawls on hands and knees.....                | 1.....        | 1.....                | 1.....                 | 2.....                 | 2.....                 | 2.....                 | 2.....                 |
| Sampling and readings.....                    |               |                       | 2.....                 |                        |                        | 2.....                 | 2.....                 |
| Runs at 9.7 km. (6 miles) per hour.....       |               |                       |                        | 1.....                 | 1.....                 | 1.....                 | 1.....                 |
| Walks at 4.8 km. (3 miles) per hour.....      |               |                       |                        |                        |                        | 8.....                 | 10.....                |
| Pulls 20 kg. (45 pound) weight to 5 feet..... |               |                       | 30 times in 2 minutes. |                        | 60 times in 6 minutes. | 60 times in 6 minutes. | 60 times in 6 minutes. |
| Sampling and readings.....                    |               |                       |                        | 2.....                 |                        | 2.....                 | 2.....                 |
| Walks at 4.8 km. (3 miles) per hour.....      |               |                       | 1.....                 |                        | 3.....                 | 4.....                 | 10.....                |
| Lies on side.....                             |               |                       |                        |                        |                        | 2.....                 | 4.....                 |
| Lies on back.....                             |               |                       |                        |                        |                        | 2.....                 | 1.....                 |
| Sampling and readings.....                    |               |                       |                        |                        | 2.....                 | 2.....                 | 2.....                 |

<sup>1</sup> Total test time for Test 3 for 2-hour, 3-hour, and 4-hour apparatus is 2 hours.

Perform test No. 3 for 1 hr. apparatus; then perform test No. 1 for 1 hour apparatus.

# RULES AND REGULATIONS

6257

TABLE 4.—DURATION AND SEQUENCE OF SPECIFIC ACTIVITIES FOR TEST 4, IN MINUTES  
(30 CFR Part 11, Subpart II, § 11.35, et seq.)

| Activity                                                                      | Service time— |                        |                        |                        |                        |                        |                        |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
|-------------------------------------------------------------------------------|---------------|------------------------|------------------------|------------------------|------------------------|------------------------|------------------------|--------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|                                                                               | 3 minutes     | 5 minutes              | 10 minutes             | 15 minutes             | 30 minutes             | 45 minutes             | 1 hour                 | 2 hours                                                                                                                                    | 3 hours                                                                                                                              | 4 hours                                                                                                                                                               |
| Sampling and readings.....                                                    |               |                        |                        | 2.....                 | 2.....                 | 2.....                 | 2.....                 | Perform test No. 1 for 30-minute apparatus; then perform test No. 4 for 1-hour apparatus; then perform test No. 1 for 30-minute apparatus. | Perform test No. 1 for 1-hour apparatus; then perform test No. 4 for 1-hour apparatus; then perform test No. 1 for 1-hour apparatus. | Perform test No. 1 for 1-hour apparatus; then perform test No. 4 for 1-hour apparatus; then perform test No. 1 for 1-hour apparatus twice (i.e., two one-hour tests). |
| Walks at 4.8 km. (3 miles) per hour.....                                      |               |                        |                        | 1.....                 | 2.....                 | 2.....                 | 2.....                 |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Climbs vertical treadmill <sup>1</sup> (or equivalent).....                   | 1.....        | 1.....                 | 1.....                 | 1.....                 | 1.....                 | 1.....                 | 1.....                 |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Walks at 4.8 km. (3 miles) per hour.....                                      |               | 1.....                 | 1.....                 | 1.....                 | 2.....                 | 2.....                 | 2.....                 |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Pulls 20 kg. (45 pound) weight to 5 feet.....                                 |               | 30 times in 2 minutes. | 30 times in 2 minutes. | 30 times in 2 minutes. | 60 times in 5 minutes. | 60 times in 5 minutes. | 60 times in 5 minutes. |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Walks at 4.8 km. (3 miles) per hour.....                                      |               |                        | 1.....                 | 1.....                 | 1.....                 | 1.....                 | 1.....                 |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Carries 23 kg. (50 pound) weight over overcast.....                           |               |                        |                        | 1 time in 1 minute.    | 1 time in 1 minute.    | 2 times in 3 minutes.  | 4 times in 8 minutes.  |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Sampling and readings.....                                                    |               |                        | 2.....                 |                        | 2.....                 | 2.....                 | 2.....                 |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Walks at 4.8 km. (3 miles) per hour.....                                      |               |                        |                        | 1.....                 | 3.....                 | 3.....                 | 4.....                 |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Runs at 9.7 km. (6 miles) per hour.....                                       |               |                        |                        | 1.....                 | 1.....                 | 1.....                 | 1.....                 |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Carries 23 kg. (50 pound) weight over overcast.....                           |               |                        |                        | 1 time in 1 minute.    | 1 time in 1 minute.    | 2 times in 3 minutes.  | 4 times in 8 minutes.  |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Pulls 20 kg. (45 pound) weight to 5 feet.....                                 |               | 15 times in 1 minute.  |                        | 15 times in 1 minute.  | 60 times in 5 minutes. | 30 times in 2 minutes. | 36 times in 3 minutes. |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Sampling and readings.....                                                    |               |                        |                        | 2.....                 | 2.....                 | 2.....                 | 2.....                 |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Walks at 4.8 km. (3 miles) per hour.....                                      |               |                        | 1.....                 |                        | 2.....                 | 2.....                 | 6.....                 |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Pulls 20 kg. (45 pound) weight to 5 feet.....                                 |               |                        |                        |                        | 60 times in 5 minutes. | 60 times in 5 minutes. | 60 times in 5 minutes. |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Carries 20 kg. (45 pound) weight and walks at 4.8 km. (3 miles) per hour..... |               |                        |                        |                        |                        | 3.....                 | 3.....                 |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |
| Sampling and readings.....                                                    |               |                        |                        |                        |                        | 2.....                 | 2.....                 |                                                                                                                                            |                                                                                                                                      |                                                                                                                                                                       |

<sup>1</sup> Treadmill shall be inclined 15° from vertical and operated at a speed of 30 cm. (1 foot) per second.

## Subpart I—Gas Masks

### § 11.90 Gas masks; description.

(a) Gas masks including all completely assembled air purifying masks which are designed for use as respiratory protection during entry into and escape or escape only from hazardous atmospheres containing adequate oxygen to support life are described as follows:

(1) *Front-mounted or back-mounted gas mask.* A gas mask which consists of a full facepiece, a breathing tube, a canister at the front or back, a canister harness, and associated connections.

(2) *Type "N" front-mounted or back-mounted gas mask.* A gas mask specifically designed to protect against acid gases, ammonia, carbon monoxide, organic vapors, and particulate contaminants which consists of a full facepiece, breathing tube, a canister at the front or back, a canister harness, and associated connections.

(3) *Chin-style gas mask.* A gas mask which consists of a full facepiece, a canister which is usually attached to the facepiece, and associated connections.

(4) *Escape gas mask.* A gas mask designed for use during escape only from hazardous atmospheres which consists of a half-mask facepiece or mouthpiece, a canister, and associated connections.

(b) Gas masks shall be further described according to the specific gases or vapors against which they are designed to provide respiratory protection, as follows:

| Type of front-mounted or back-mounted gas mask: | Maximum use concentration, percent by volume |
|-------------------------------------------------|----------------------------------------------|
| Acid gas <sup>1, 2, 3</sup> .....               | * 2                                          |
| Ammonia <sup>1</sup> .....                      | 3                                            |
| Carbon monoxide <sup>1</sup> .....              | 2                                            |
| Organic vapors <sup>1, 4</sup> .....            | * 2                                          |
| Type of chin-style gas mask:                    | Maximum use concentration, percent by volume |
| Acid gas <sup>1, 2, 3</sup> .....               | * 0.5                                        |
| Ammonia <sup>1</sup> .....                      | .5                                           |
| Organic vapors <sup>1, 4</sup> .....            | * .5                                         |
| Type of escape gas mask:                        | Maximum use concentration, parts per million |
| Acid gas <sup>1, 2, 3, 4</sup> .....            | * 1,000                                      |
| Ammonia <sup>1</sup> .....                      | 5,000                                        |
| Carbon monoxide <sup>1</sup> .....              | 10,000                                       |
| Organic vapors <sup>1, 4</sup> .....            | * 5,000                                      |

<sup>1</sup> Approval may be for acid gases or organic vapors as a class or for specific acid gases, ammonia, or organic vapors. Approval may also be granted for combinations of acid gases, organic vapors, and other gases and vapors.

<sup>2</sup> Not for use against acid gases or organic vapors with poor warning properties or which generate high heats of reaction with solvent materials in the canister.

<sup>3</sup> Suggested maximum use concentrations are lower than these for some acid gases and organic vapors.

<sup>4</sup> Eye protection may be required in certain concentrations of acid gases, ammonia, and organic vapors.

(c) Gas masks for respiratory protection against gases and vapors other than those specified in paragraph (b) of this section may be approved. The applicant shall submit a request for approval, in writing, to the Bureau of Mines, Approval and Testing, 4800 Forbes Avenue, Pittsburgh, PA 15213, listing the gas or vapor and suggested maximum use concentration for the specific type of gas mask. The Bureau and the Institute will consider the application and accept or reject the application on the basis of effect on the wearer's health and safety and any field experience in use of gas masks for such exposures. If the application is accepted the Bureau will test such gas mask in accordance with the requirements of this subpart.

### § 11.91 Gas masks; required components.

(a) Each gas mask described in § 11.90 shall, where its design requires, contain the following component parts:

- (1) Facepiece or mouthpiece and noseclip;
- (2) Canister or cartridge;
- (3) Canister harness;
- (4) External check valve; and
- (5) Breathing tube.

(b) The components of each gas mask shall meet the minimum construction requirements set forth in Subpart G of this part.

**§ 11.92 Canisters and cartridges in parallel; resistance requirements.**

Where two or more canisters or cartridges are used in parallel, their resistance to airflow shall be essentially equal.

**§ 11.93 Canisters and cartridges; color and markings; requirements.**

The color and markings of all canisters and cartridges or labels shall conform with the requirements of the American National Standard for Identification of Gas Mask Canisters, K13.1, obtainable from American National Standards Institute, Inc., 1430 Broadway, New York, NY 10018.

**§ 11.94 Filters used with canisters and cartridges; location; replacement.**

(a) Particulate matter filters used in conjunction with a canister or cartridge shall be located on the inlet side of the canister or cartridge.

(b) Filters shall be incorporated in or firmly attached to the canister or cartridge and each filter assembly shall, where applicable, be designed to permit its easy removal from and replacement in the canister or cartridge.

**§ 11.95 Breathing tubes; minimum requirements.**

(a) Flexible breathing tubes used in conjunction with gas masks shall be designed and constructed to prevent:

- (1) Restriction of free head movement;
- (2) Disturbance of the fit of facepieces or mouthpieces;
- (3) Interference with the wearer's activities; and,
- (4) Shutoff of airflow due to kinking, or from chin or arm pressure.

**§ 11.96 Harnesses; installation and construction; minimum requirements.**

(a) Each gas mask shall, where necessary, be equipped with a suitable harness designed and constructed to hold the components of the gas mask in position against the wearer's body.

(b) Harnesses shall be designed and constructed to permit easy removal and replacement of gas mask parts, and where applicable, provide for holding a full facepiece in the ready position when not in use.

**§ 11.97 Gas mask containers; minimum requirements.**

(a) Gas masks shall be equipped with a substantial, durable container bearing markings which show the applicant's name, the type and commercial designation of mask it contains and all appropriate approval labels.

(b) Containers for gas masks shall be designed and constructed to permit easy removal of the mask.

**§ 11.98 Half-mask facepieces, full facepieces and mouthpieces; fit; minimum requirements.**

(a) Half-mask facepieces and full facepieces shall be designed and constructed to fit persons with various facial shapes and sizes either: (1) By providing more than one facepiece size, or (2)

by providing one facepiece size which will fit varying facial shapes and sizes.

(b) Full facepieces shall provide for optional use of corrective spectacles or lenses, which shall not reduce the respiratory protective qualities of the gas mask.

(c) Half-mask facepieces shall not interfere with the fit of common industrial safety spectacles, as determined by the Bureau's facepiece tests in § 11.102-3.

(d) Gas masks with mouthpieces shall be equipped with noseclips which are securely attached to the mouthpiece or gas mask and provide an airtight seal.

(e) Facepieces shall be designed to prevent eyepiece fogging.

**§ 11.99 Facepieces; eyepieces; minimum requirements.**

(a) Full facepieces shall be designed and constructed to provide adequate vision which is not distorted by the eyepiece.

(b) All eyepieces shall be designed and constructed to meet the impact and penetration requirements specified in Federal Specification, Mask, Air Line: and Respirator, Air Filtering, Industrial, GGG-M-125d, October 11, 1965.

**§ 11.100 Inhalation and exhalation valves; minimum requirements.**

(a) Inhalation and exhalation valves shall be provided where necessary and protected against damage and distortion.

(b) Inhalation valves shall be designed and constructed to prevent excessive exhaled air from adversely affecting cartridges, canisters, and filters.

(c) Exhalation valves shall be protected against external influence, and designed and constructed to prevent inward leakage of contaminated air.

**§ 11.101 Head harnesses; minimum requirements.**

(a) Facepieces shall be equipped with adjustable and replaceable head harnesses, designed and constructed to provide adequate tension during use and an even distribution of pressure over the entire area in contact with the face.

(b) Mouthpieces shall be equipped, where applicable, with adjustable and replaceable harnesses designed and constructed to hold the mouthpiece in place.

**§ 11.102 Gas masks; performance requirements; general.**

Gas masks and the individual components of each such device shall, as appropriate, meet the requirements for performance and protection specified in the tests described in §§ 11.102-1 through 11.102-5.

**§ 11.102-1 Breathing resistance test; minimum requirements.**

(a) Resistance to airflow will be measured in the facepiece or mouthpiece of a gas mask mounted on a breathing machine both before and after each test conducted in accordance with §§ 11.102-3, 11.102-4, and 11.102-5, with air flowing at a continuous rate of 85 liters per minute.

(b) The maximum allowable resistance requirements for gas masks are as follows:

| Type of gas mask <sup>1</sup>                                         | MAXIMUM RESISTANCE<br>(mm. water-column height) |       |            |
|-----------------------------------------------------------------------|-------------------------------------------------|-------|------------|
|                                                                       | Inhalation                                      |       | Exhalation |
|                                                                       | Initial                                         | Final |            |
| Front-mounted or back-mounted (without particulate filter).....       | 60                                              | 75    | 20         |
| Front-mounted or back-mounted (with approved particulate filter)..... | 70                                              | 85    | 20         |
| Chin-style (without particulate filter).....                          | 40                                              | 55    | 20         |
| Chin-style (with approved particulate filter).....                    | 65                                              | 80    | 20         |
| Escape (without particulate filter).....                              | 60                                              | 75    | 20         |
| Escape (with approved particulate filter).....                        | 70                                              | 85    | 20         |

<sup>1</sup> Measured at end of the service life specified in Tables 5, 6, and 7.

**§ 11.102-2 Exhalation valve leakage test.**

(a) Dry exhalation valves and valve seats will be subjected to a suction of 25 mm. water-column height while in a normal operating position.

(b) Leakage between the valve and valve seat shall not exceed 30 milliliters per minute.

**§ 11.102-3 Facepiece tests; minimum requirements.**

(a) The complete gas mask will be fitted to the faces of persons having varying facial shapes and sizes.

(b) Where the applicant specifies a facepiece size or sizes for the gas mask together with the approximate measurements of faces they are designed to fit, the Bureau will insure that test subjects suit such facial measurements.

(c) Any gas mask parts which must be removed to perform the facepiece or mouthpiece fit test shall be replaceable without special tools and without disturbing the facepiece or mouthpiece fit.

(d) The facepiece or mouthpiece fit test, using positive or negative pressure recommended by the applicant and described in his instructions will be used before each test specified in paragraph (e) of this section, and in § 11.102-4.

(e) (1) Each wearer will enter a chamber containing 100 p.p.m. isoamyl acetate vapor for a half-mask facepiece and 1,000 p.p.m. isoamyl acetate vapor for a full facepiece or mouthpiece.

(2) The facepiece or mouthpiece may be adjusted, if necessary, in the test chamber before starting the tests.

(3) Each wearer will remain in the chamber for 8 minutes while performing the following activities:

- (i) Two minutes, nodding and turning head;
- (ii) Two minutes, callisthenic arm movements;
- (iii) Two minutes, running in place, and
- (iv) Two minutes, pumping with a tire pump into a 28 liter (1 cubic foot) container.

(4) Each wearer shall not detect the odor of isoamyl acetate during the test.

§ 11.102-4 Dust, fume, mist, and smoke tests; canisters containing filters; minimum requirements.

(a) Gas mask canisters containing filters for protection against dusts, fumes, mists, and smokes in combination with gases, vapors, or gases and vapors, will be tested as prescribed in § 11.140.

(b) Gas mask canisters designed for protection against smokes will be tested in an atmospheric concentration of 100 micrograms of dioctyl phthalate per liter of air at continuous flow rates of (1) 32 liters per minute, and (2) 85 liters per minute for a period of 5 to 10 seconds, and the DOP leakage through the canister shall not exceed 0.03 percent of the test concentration.

§ 11.102-5 Canister bench tests; minimum requirements.

(a) (1) Bench tests, except for carbon monoxide tests, will be made on an apparatus that allows the test atmosphere at  $50 \pm 5$  percent relative humidity and room temperature ( $25 \pm 2.5^\circ \text{C}$ ) to enter the canister continuously at concentrations and rates of flow specified in Tables 5, 6, and 7.

(2) Three canisters will be removed from containers and tested as received from the applicant.

(3) Two canisters, other than those described in paragraph (a) (2) of this section, will be equilibrated at room temperature by passing 25 percent relative humidity air through them at 64 liters per minute for 6 hours.

(4) Two canisters, other than those described in paragraphs (a) (2) and (3) of this section, will be equilibrated at room temperature by passing 85 percent relative humidity air through them at 64 liters per minute for 6 hours.

(5) The equilibrated canisters will be resealed, kept in an upright position at room temperature, and tested within 18 hours.

(b) Front-mounted and back-mounted gas mask canisters will be tested and shall meet the minimum requirements set forth in Table 5.

(c) (1) Front-mounted and back-mounted canisters designated as Type N canisters shall have a window or other indicator to warn the gas mask wearer when the canister will no longer satisfactorily remove carbon monoxide from the inhaled air.

(2) Other types of front- and back-mounted canisters may also be equipped with a window or other indicator to warn of imminent leakage of other gases or vapors.

(3) The window indicator canisters will be tested as regular canisters, but shall show a satisfactory indicator change or other warning before the allowable canister penetration has occurred.

(d) Chin-style gas mask canisters shall meet the minimum requirements set forth in Table 6.

(e) Escape gas mask canisters shall meet the minimum requirements set forth in Table 7.

TABLE 5.—CANISTER BENCH TESTS AND REQUIREMENTS FOR FRONT AND BACK-MOUNTED GAS MASK CANISTERS  
(30 CFR Part 11, Subpart I, § 11.102-5)

| Canister type        | Test condition    | Test atmosphere  |                       |                   | Number of tests | Maximum allowable penetration, p.p.m. | Minimum service life, minutes <sup>1</sup> |
|----------------------|-------------------|------------------|-----------------------|-------------------|-----------------|---------------------------------------|--------------------------------------------|
|                      |                   | Gas or vapor     | Concentration, p.p.m. | Flow rate, l.p.m. |                 |                                       |                                            |
| Acid gas.....        | As received.....  | SO <sub>2</sub>  | 20,000                | 64                | 3               | 5                                     | 12                                         |
|                      |                   | Cl <sub>2</sub>  | 20,000                | 64                | 3               | 5                                     | 12                                         |
|                      |                   | NO <sub>2</sub>  | 20,000                | 64                | 3               | 5                                     | 12                                         |
|                      | Equilibrated..... | SO <sub>2</sub>  | 20,000                | 32                | 4               | 5                                     | 12                                         |
|                      |                   | Cl <sub>2</sub>  | 20,000                | 32                | 4               | 5                                     | 12                                         |
|                      |                   | NO <sub>2</sub>  | 20,000                | 32                | 4               | 5                                     | 12                                         |
| Organic vapors.....  | As received.....  | CCl <sub>4</sub> | 20,000                | 64                | 3               | 5                                     | 12                                         |
|                      | Equilibrated..... | CCl <sub>4</sub> | 20,000                | 32                | 4               | 5                                     | 12                                         |
| Ammonia.....         | As received.....  | NH <sub>3</sub>  | 30,000                | 64                | 3               | 50                                    | 12                                         |
|                      | Equilibrated..... | NH <sub>3</sub>  | 30,000                | 32                | 4               | 50                                    | 12                                         |
| Carbon monoxide..... | As received.....  | CO               | 20,000                | 64                | 2               | (7)                                   | 60                                         |
|                      |                   | CO               | 5,000                 | 32                | 3               | (7)                                   | 60                                         |
|                      |                   | CO               | 3,000                 | 32                | 3               | (7)                                   | 60                                         |
|                      |                   | CO               | 20,000                | 64                | 3               | 5                                     | 6                                          |
| Type N.....          | As received.....  | SO <sub>2</sub>  | 20,000                | 64                | 3               | 5                                     | 6                                          |
|                      |                   | Cl <sub>2</sub>  | 20,000                | 64                | 3               | 5                                     | 6                                          |
|                      |                   | NO <sub>2</sub>  | 20,000                | 64                | 3               | 5                                     | 6                                          |
|                      |                   | CCl <sub>4</sub> | 20,000                | 64                | 3               | 5                                     | 6                                          |
|                      |                   | NH <sub>3</sub>  | 30,000                | 64                | 3               | 50                                    | 6                                          |
|                      |                   | CO               | 20,000                | 64                | 2               | (7)                                   | 60                                         |
|                      |                   | CO               | 5,000                 | 32                | 3               | (7)                                   | 60                                         |
|                      | Equilibrated..... | SO <sub>2</sub>  | 20,000                | 32                | 4               | 5                                     | 6                                          |
|                      |                   | Cl <sub>2</sub>  | 20,000                | 32                | 4               | 5                                     | 6                                          |
|                      |                   | NO <sub>2</sub>  | 20,000                | 32                | 4               | 5                                     | 6                                          |
|                      |                   | CCl <sub>4</sub> | 20,000                | 32                | 4               | 5                                     | 6                                          |
|                      |                   | NH <sub>3</sub>  | 30,000                | 32                | 4               | 50                                    | 6                                          |
|                      |                   | CO               | 20,000                | 32                | 4               | 5                                     | 6                                          |
|                      |                   | CO               | 5,000                 | 32                | 4               | 5                                     | 6                                          |

<sup>1</sup> Minimum life will be determined at the indicated penetration.

<sup>2</sup> Relative humidity of test atmosphere will be  $95 \pm 3$  percent; temperature of test atmosphere will be  $25 \pm 2.5^\circ \text{C}$ .

<sup>3</sup> Maximum allowable CO penetration will be 365 cc. during the minimum life. The penetration shall not exceed 500 p.p.m. during this time.

<sup>4</sup> Relative humidity of test atmosphere will be  $95 \pm 3$  percent; temperature of test atmosphere entering the test fixture will be  $0 \pm 2.5^\circ \text{C}$  to  $0^\circ \text{C}$ .

TABLE 6.—CANISTER BENCH TESTS AND REQUIREMENTS FOR CHIN-STYLE GAS MASK CANISTERS  
(30 CFR Part 11, Subpart I, § 11.102-5)

| Canister type       | Test condition    | Test atmosphere  |                       |                   | Number of tests | Maximum allowable penetration, p.p.m. | Minimum service life, minutes <sup>1</sup> |
|---------------------|-------------------|------------------|-----------------------|-------------------|-----------------|---------------------------------------|--------------------------------------------|
|                     |                   | Gas or vapor     | Concentration, p.p.m. | Flow rate, l.p.m. |                 |                                       |                                            |
| Acid gas.....       | As received.....  | SO <sub>2</sub>  | 5,000                 | 64                | 3               | 5                                     | 12                                         |
|                     |                   | Cl <sub>2</sub>  | 5,000                 | 64                | 3               | 5                                     | 12                                         |
|                     |                   | NO <sub>2</sub>  | 5,000                 | 64                | 3               | 5                                     | 12                                         |
|                     | Equilibrated..... | SO <sub>2</sub>  | 5,000                 | 32                | 4               | 5                                     | 12                                         |
|                     |                   | Cl <sub>2</sub>  | 5,000                 | 32                | 4               | 5                                     | 12                                         |
|                     |                   | NO <sub>2</sub>  | 5,000                 | 32                | 4               | 5                                     | 12                                         |
| Organic vapors..... | As received.....  | CCl <sub>4</sub> | 5,000                 | 64                | 3               | 5                                     | 12                                         |
|                     | Equilibrated..... | CCl <sub>4</sub> | 5,000                 | 32                | 4               | 5                                     | 12                                         |
| Ammonia.....        | As received.....  | NH <sub>3</sub>  | 5,000                 | 64                | 3               | 50                                    | 12                                         |
|                     | Equilibrated..... | NH <sub>3</sub>  | 5,000                 | 32                | 4               | 50                                    | 12                                         |

<sup>1</sup> Minimum life will be determined at the indicated penetration.

TABLE 7.—CANISTER BENCH TESTS AND REQUIREMENTS FOR ESCAPE GAS MASK CANISTERS  
(30 CFR Part 11, Subpart I, § 11.102-5)

| Canister type        | Test condition    | Test atmosphere  |                       |                   | Number of tests | Maximum allowable penetration, p.p.m. | Minimum service life, minutes <sup>1</sup> |
|----------------------|-------------------|------------------|-----------------------|-------------------|-----------------|---------------------------------------|--------------------------------------------|
|                      |                   | Gas or vapor     | Concentration, p.p.m. | Flow rate, l.p.m. |                 |                                       |                                            |
| Acid gas.....        | As received.....  | SO <sub>2</sub>  | 5,000                 | 64                | 3               | 5                                     | 12                                         |
|                      |                   | Cl <sub>2</sub>  | 5,000                 | 64                | 3               | 5                                     | 12                                         |
|                      |                   | NO <sub>2</sub>  | 5,000                 | 64                | 3               | 5                                     | 12                                         |
|                      | Equilibrated..... | SO <sub>2</sub>  | 5,000                 | 32                | 4               | 5                                     | 12                                         |
|                      |                   | Cl <sub>2</sub>  | 5,000                 | 32                | 4               | 5                                     | 12                                         |
|                      |                   | NO <sub>2</sub>  | 5,000                 | 32                | 4               | 5                                     | 12                                         |
| Organic vapors.....  | As received.....  | CCl <sub>4</sub> | 5,000                 | 64                | 3               | 5                                     | 12                                         |
|                      | Equilibrated..... | CCl <sub>4</sub> | 5,000                 | 32                | 4               | 5                                     | 12                                         |
| Ammonia.....         | As received.....  | NH <sub>3</sub>  | 5,000                 | 64                | 3               | 50                                    | 12                                         |
|                      | Equilibrated..... | NH <sub>3</sub>  | 5,000                 | 32                | 4               | 50                                    | 12                                         |
| Carbon monoxide..... | As received.....  | CO               | 10,000                | 32                | 2               | (7)                                   | 60                                         |
|                      |                   | CO               | 5,000                 | 32                | 3               | (7)                                   | 60                                         |
|                      |                   | CO               | 3,000                 | 32                | 3               | (7)                                   | 60                                         |

<sup>1</sup> Minimum life will be determined at the indicated penetration.

<sup>2</sup> Relative humidity of test atmosphere will be  $95 \pm 3$  percent; temperature of test atmosphere will be  $25 \pm 2.5^\circ \text{C}$ .

<sup>3</sup> Maximum allowable CO penetration will be 365 cc. during the minimum life. The penetration shall not exceed 500 p.p.m. during this time.

<sup>4</sup> If effluent temperature exceeds  $100^\circ \text{C}$ . during this test, the escape gas mask shall be equipped with an effective heat exchanger.

<sup>5</sup> Relative humidity of test atmosphere will be  $95 \pm 3$  percent; temperature of test atmosphere entering the test fixture will be  $0 \pm 2.5^\circ \text{C}$  to  $0^\circ \text{C}$ .

**Subpart J—Supplied-Air Respirators****§ 11.110 Supplied-air respirators; description.**

(a) Supplied-air respirators, including all completely assembled respirators designed for use as respiratory protection during entry into and escape from hazardous atmospheres are described as follows:

(1) *Type "A" supplied-air respirators.* A hose mask respirator, for entry into and escape from hazardous atmospheres, which consists of a motor-driven or hand-operated blower that permits the free entrance of air when the blower is not operating, a strong large-diameter hose having a low resistance to airflow, a harness to which the hose and the lifeline are attached and a tight-fitting facepiece.

(2) *Type "AE" supplied-air respirators.* A Type "A" supplied-air respirator equipped with additional devices designed to protect the wearer's head and neck against impact and abrasion from rebounding abrasive material, and with shielding material such as plastic, glass, woven wire, sheet metal, or other suitable material to protect the window(s) of facepieces, hoods, and helmets which do not unduly interfere with the wearer's vision and permit easy access to the external surface of such window(s) for cleaning.

(3) *Type "B" supplied-air respirators.* A hose mask respirator, for entry into and escape from atmospheres not immediately dangerous to life or health, which consists of a strong large-diameter hose with low resistance to airflow through which the user draws inspired air by means of his lungs alone, a harness to which the hose is attached, and a tight-fitting facepiece.

(4) *Type "BE" supplied-air respirators.* A type "B" supplied-air respirator equipped with additional devices designed to protect the wearer's head and neck against impact and abrasion from rebounding abrasive material, and with shielding material such as plastic, glass, woven wire, sheet metal, or other suitable material to protect the window(s) of facepieces, hoods, and helmets which do not unduly interfere with the wearer's vision and permit easy access to the external surface of such window(s) for cleaning.

(5) *Type "C" supplied-air respirators.* An airline respirator, for entry into and escape from atmospheres not immediately dangerous to life or health, which consists of a source of respirable breathing air, a hose, a detachable coupling, a control valve, orifice, a demand valve or pressure demand valve, an arrangement for attaching the hose to the wearer, and a facepiece, hood, or helmet.

(6) *Type "CE" supplied-air respirators.* A type "C" supplied-air respirator equipped with additional devices designed to protect the wearer's head and neck against impact and abrasion from rebounding abrasive material, and with shielding material such as plastic, glass, woven wire, sheet metal, or other suitable material to protect the window(s) of facepieces, hoods, and helmets which

do not unduly interfere with the wearer's vision and permit easy access to the external surface of such window(s) for cleaning.

**§ 11.111 Supplied-air respirators; required components.**

(a) Each supplied-air respirator described in § 11.110 shall, where its design requires, contain the following component parts:

- (1) Facepiece, hood, or helmet;
- (2) Air supply valve, orifice, or demand or pressure-demand regulator;
- (3) Hand operated or motor driven air blower;
- (4) Air supply hose;
- (5) Detachable couplings;
- (6) Flexible breathing tube; and
- (7) Respirator harness.

(b) The component parts of each supplied-air respirator shall meet the minimum construction requirements set forth in Subpart G of this part.

**§ 11.112 Breathing tubes; minimum requirements.**

(a) Flexible breathing tubes used in conjunction with supplied-air respirators shall be designed and constructed to prevent:

- (1) Restriction of free head movement;
- (2) Disturbance of the fit of facepieces, mouthpieces, hoods, or helmets;
- (3) Interference with the wearer's activities; and
- (4) Snuffoff of airflow due to kinking, or from chin or arm pressure.

**§ 11.113 Harnesses; installation and construction; minimum requirements.**

(a) Each supplied-air respirator shall, where necessary, be equipped with a suitable harness designed and constructed to hold the components of the respirator in position against the wearer's body.

(b) Harnesses shall be designed and constructed to permit easy removal and replacement of respirator parts, and where applicable, provide for holding a full facepiece in the ready position when not in use.

**§ 11.114 Respirator containers; minimum requirements.**

Supplied-air respirators shall be equipped with a substantial, durable container bearing markings which show the applicant's name, the type and commercial designation of the respirator it contains, and all appropriate approval labels.

**§ 11.115 Half-mask facepieces, full facepieces, hoods, and helmets; fit; minimum requirements.**

(a) Half-mask facepieces and full facepieces shall be designed and constructed to fit persons with various facial shapes and sizes either (1) by providing more than one facepiece size, or (2) by providing one facepiece size which will fit varying facial shapes and sizes.

(b) Full facepieces shall provide for optional use of corrective spectacles or lenses, which shall not reduce the respiratory protective qualities of the respirator.

(c) Hoods and helmets shall be designed and constructed to fit persons with various head sizes, provide for the optional use of corrective spectacles or lenses, and insure against any restriction of movement by the wearer.

(d) Facepieces, hoods, and helmets shall be designed to prevent eyepiece fogging.

**§ 11.116 Facepieces, hoods, and helmets; eyepieces; minimum requirements.**

(a) Facepieces, hoods, and helmets shall be designed and constructed to provide adequate vision which is not distorted by the eyepiece.

(b) All eyepieces except those on Types B, BE, C, and CE supplied-air respirators shall be designed and constructed to meet the impact and penetration requirements specified in Federal Specification, Mask, Air Line, and Respirator, Air Filtering, Industrial GGG-M-125d, October 11, 1965.

(c) (1) The eyepieces of AE, BE, and CE type supplied-air respirators shall be shielded by plastic, glass, woven wire, sheet metal, or other suitable material which does not interfere with the vision of the wearer.

(2) Shields shall be mounted and attached to the facepiece to provide easy access to the external surface of the eyepiece for cleaning.

**§ 11.117 Inhalation and exhalation valves; check valves; minimum requirements.**

(a) Inhalation and exhalation valves shall be provided where necessary and protected against distortion.

(b) Exhalation valves shall be:

- (1) Protected against damage and external influence; and
- (2) Designed and constructed to prevent inward leakage of contaminated air.

(c) Check valves designed and constructed to allow airflow toward the facepiece only shall be provided in the connections to the facepiece or in the hose fitting near the facepiece of all Type A, AE, B, and BE supplied-air respirators.

**§ 11.118 Head harnesses; minimum requirements.**

Facepieces shall be equipped with adjustable and replaceable head harnesses which are designed and constructed to provide adequate tension during use, and an even distribution of pressure over the entire area in contact with the face.

**§ 11.119 Head and neck protection; supplied-air respirators; minimum requirements.**

Type AE, BE, and CE supplied-air respirators shall be designed and constructed to provide protection against impact and abrasion from rebounding abrasive materials to the wearer's head and neck.

**§ 11.120 Air velocity and noise levels; hoods and helmets; minimum requirements.**

Noise levels generated by the respirator will be measured inside the hood or helmet at maximum airflow obtainable

within pressure and hose length requirements and shall not exceed 80 dBA.

**§ 11.121 Breathing gas; minimum requirements.**

(a) Breathing gas used to supply supplied-air respirators shall be respirable breathing air and contain no less than 19.5 volume-percent of oxygen.

(b) Compressed, gaseous breathing air shall meet the applicable minimum grade requirements for Type I gaseous air set forth in the Compressed Gas Association Commodity Specification for Air, G-7.1 (Grade D or higher quality).

(c) Compressed, liquefied breathing air shall meet the applicable minimum grade requirements for Type II liquid air set forth in the Compressed Gas Association Commodity Specification for Air, G-7.1 (Grade B or higher quality).

**§ 11.122 Air supply source; hand-operated or motor driven air blowers; Type A supplied-air respirators; minimum requirements.**

(a) Blowers shall be designed and constructed to deliver an adequate amount of air to the wearer with either direction of rotation, unless constructed to permit rotation in one direction only, and to permit the free entrance of air to the hose when the blower is not operated.

(b) No multiple systems, whereby more than one user is supplied by one blower, will be approved, unless each hose line is connected directly to a manifold at the blower.

**§ 11.123 Terminal fittings or chambers; Type B supplied-air respirators; minimum requirements.**

(a) Blowers or connections to air supplies providing positive pressures shall not be approved for use on Type B supplied-air respirators.

(b) Terminal fittings or chambers employed in Type B supplied-air respirators, shall be:

(1) Installed in the inlet of the hose;

(2) Designed and constructed to provide for the drawing of air through corrosion resistant material arranged so as to be capable of removing material larger than 0.149 mm. in diameter (149 micrometers, 100-mesh, U.S. Standard sieve).

(3) Installed to provide a means for fastening or anchoring the fitting or chamber in a fixed position in a zone of respirable air.

**§ 11.124 Supplied-air respirators; performance requirements; general.**

Supplied-air respirators and the individual components of each such device shall, as appropriate, meet the requirements for performance and protection specified in the tests described in §§ 11.124-1 through 11.124-24.

**§ 11.124-1 Hand-operated blower test; minimum requirements.**

(a) Hand-operated blowers shall be tested by attaching them to a mechanical drive and operating them 6 to 8 hours daily for a period of 100 hours at a speed necessary to deliver 50 liters of air per

minute through each completely assembled respirator. Each respirator shall be equipped with the maximum length of hose with which the device is to be approved and the hose shall be connected to each blower or manifold outlet designed for hose connections.

(b) The crank speed of the hand-operated blower shall not exceed 50 revolutions per minute in order to deliver the required 50 liters of air per minute to each facepiece.

(c) The power required to deliver 50 liters of air per minute to each wearer through the maximum length of hose shall not exceed one-fiftieth horsepower, and the torque shall not exceed a force of 2.3 kg. (5 pounds) on a 20 cm. (8-inch) crank, as defined in § 11.124-3.

(d) The blower shall operate throughout the period without failure or indication of excessive wear of bearings or other working parts.

**§ 11.124-2 Motor-operated blower test; minimum requirements.**

(a) Motor-operated blowers shall be tested by operating them at their specified running speed 6 to 8 hours daily for a period of 100 hours when assembled with the kind and maximum length of hose for which the device is to be approved and when connected to each blower or manifold outlet designed for hose connections.

(b) The connection between the motor and the blower shall be so constructed that the motor may be disengaged from the blower when the blower is operated by hand.

(c) The blower shall operate throughout the period without failure or indication of excessive wear of bearings or other working parts.

(d) Where a blower, which is ordinarily motor driven, is operated by hand, the power required to deliver 50 liters of air per minute to each wearer through the maximum length of hose shall not exceed one-fiftieth horsepower, and the torque shall not exceed a force of 2.3 kg. (5 pounds) on a 20 cm. (8-inch) crank, as defined in § 11.124-3.

(e) Where the respirator is assembled with the facepiece and 15 m. (50 feet) of the hose for which it is to be approved, and when connected to one outlet with all other outlets closed and operated at a speed not exceeding 50 revolutions of the crank per minute, the amount of air delivered into the respiratory-inlet covering shall not exceed 150 liters per minute.

**§ 11.124-3 Method of measuring the power and torque required to operate blowers.**

As shown in Figure 1, the blower crank is replaced by a wooden drum, *a* (13 cm. (5 inches) in diameter is convenient). This drum is wound with about 12 m. (40 feet) of No. 2 picture cord, *b*. A weight, *c*, of sufficient mass to rotate the blower at the desired speed is suspended from this wire cord. A mark is made on the cord about 3 to 4.5 m. (10 to 15 feet) from the weight, *c*. Another mark is placed at a measured distance (6-9 m./20-30 feet is convenient) from the first.

These are used to facilitate timing. To determine the torque or horsepower required to operate the blower, the drum is started in rotation manually at or slightly above the speed at which the power measurement is to be made. The blower is then permitted to assume constant speed, and then as the first mark on the wire leaves the drum, a stopwatch is started. The watch is stopped when the second mark leaves the drum. From these data the foot-pounds per minute and the torque may be calculated.

**§ 11.124-4 Type B supplied-air respirator; minimum requirements.**

No Type B supplied-air respirator shall be approved for use with a blower or with connection to an air supply device at positive pressures.

**§ 11.124-5 Type C supplied-air respirator, continuous flow class; minimum requirements.**

(a) Respirators tested under this section shall be approved only when they supply respirable air at the pressures and quantities required.

(b) The pressure at the inlet of the hose connection shall not exceed 863 kN/m.<sup>2</sup> (125 pounds per square inch gage).

(c) Where the pressure at any point in the supply system exceeds 863 kN/m.<sup>2</sup> (125 pounds per square inch gage), the respirator shall be equipped with a pressure-release mechanism that will prevent the pressure at the hose connection from exceeding 863 kN/m.<sup>2</sup> (125 pounds per square inch gage) under any conditions.

**§ 11.124-6 Type C supplied-air respirator, demand and pressure demand class; minimum requirements.**

(a) Respirators tested under this section shall be approved only when used to supply respirable air at the pressures and quantities required.

(b) The manufacturer shall specify the range of air pressure at the point of attachment of the air-supply hose to the air-supply system, and the range of hose length for the respirator. For example, he might specify that the respirator be used with compressed air at pressures ranging from 280-550 kN/m.<sup>2</sup> (40 to 80 pounds per square inch) with from 6 to 76 m. (15 to 250 feet) of air-supply hose.

(c) The specified air pressure at the point of attachment of the hose to the air-supply system shall not exceed 863 kN/m.<sup>2</sup> (125 pounds per square inch gage).

(d) (1) Where the pressure in the air-supply system exceeds 863 kN/m.<sup>2</sup> (125 pounds per square inch gage), the respirator shall be equipped with a pressure-release mechanism that will prevent the pressure at the point of attachment of the hose to the air-supply system from exceeding 863 kN/m.<sup>2</sup> (125 pounds per square inch gage).

(2) The pressure-release mechanism shall be set to operate at a pressure not more than 20 percent above the manufacturer's highest specified pressure. For example, if the highest specified pressure is 863 kN/m.<sup>2</sup> (125 pounds per square inch), the pressure-release mechanism

would be set to operate at a maximum of 1,035 kN/m.<sup>2</sup> (150 pounds per square inch).

**§ 11.124-7 Air-supply line tests; minimum requirements.**

Air supply lines employed on Type A, Type B, and Type C supplied-air respirators shall meet the minimum test requirements set forth in Table 8.

**§ 11.124-8 Harness test; minimum requirements.**

(a) (1) Shoulder straps employed on Type A supplied-air respirators shall be tested for strength of material, joints, and seams and must separately withstand a pull of 113 kg. (250 pounds) for 30 minutes without failure.

(2) Belts, rings, and attachments for life lines must withstand a pull of 136 kg. (300 pounds) for 30 minutes without failure.

(3) The hose shall be firmly attached to the harness so as to withstand a pull of 113 kg. (250 pounds) for 30 minutes without separating, and the hose attachments shall be arranged so that the pull or drag of the hose behind an advancing wearer does not disarrange the harness or exert pull upon the facepiece.

(4) The arrangement and suitability of all harness accessories and fittings will be considered.

(b) (1) The harness employed on Type B supplied-air respirators shall not be uncomfortable, disturbing, or interfere with the movements of the wearer.

(2) The harness shall be easily adjustable to various sizes.

(3) The hose shall be attached to the harness in a manner that will withstand a pull of 45 kg. (100 pounds) for 30 minutes without separating or showing signs of failure.

(4) The design of the harness and attachment of the line shall permit dragging the maximum length of hose considered for approval over a concrete floor without disarranging the harness or exerting a pull on the facepiece.

(5) The arrangement and suitability of all harness accessories and fittings will be considered.

(c) The harness employed on Type C respirators shall be similar to that required on the Type B respirator, or, it may consist of a simple arrangement for attaching the hose to a part of the wearer's clothing in a practical manner that prevents a pull equivalent to dragging the maximum length of the hose over a concrete floor from exerting pull upon the respiratory-inlet covering.

(d) Where supplied-air respirators have a rigid or partly rigid head covering, a suitable harness shall be required to assist in holding this covering in place.

**§ 11.124-9 Breathing tube test; minimum requirements.**

(a) (1) Type A and Type B supplied-air respirators shall employ one or two flexible breathing tubes of the non-kinking type which extend from the facepiece to a connecting hose coupling attached to the belt or harness.

(2) The breathing tubes employed shall permit free head movement, insure

against closing off by kinking or by chin or arm pressure, and they shall not create a pull that will loosen the facepiece or disturb the wearer.

(b) Breathing tubes employed on Type C supplied-air respirators of the continuous flow class shall meet the minimum requirements set forth in paragraph (a) of this section, however, an extension of the connecting hose may be employed in lieu of the breathing tubes required.

(c) (1) A flexible, nonkinking type breathing tube shall: (i) Be employed on Type C supplied-air respirators of the demand and pressure-demand class; and (ii) extend from the facepiece to the demand or pressure-demand valve, except where the valve is attached directly to the facepiece.

(2) The breathing tube shall permit free head movement, insure against closing off by kinking or by chin or arm pressure, and shall not create a pull that will loosen the facepiece or disturb the wearer.

**§ 11.124-10 Airflow resistance test, Type A and Type AE supplied-air respirators; minimum requirements.**

(a) Airflow resistance will be determined when the respirator is completely assembled with the respiratory-inlet covering, the air-supply device, and the maximum length of air-supply hose coiled for one-half its length in loops 1.5 to 2.1 m. (5 to 7 feet) in diameter.

(b) The inhalation resistance, drawn at the rate of 85 liters (3 cubic feet) per minute when the blower is not operating or under any practical condition of blower operation shall not exceed the following amounts:

| Maximum length of hose for which respirator is approved |        | Maximum resistance, water column height |             |
|---------------------------------------------------------|--------|-----------------------------------------|-------------|
| Feet                                                    | Meters | Inches                                  | Millimeters |
| 75                                                      | 23     | 1.6                                     | 38          |
| 150                                                     | 46     | 2.6                                     | 64          |
| 250                                                     | 76     | 3.5                                     | 89          |
| 300                                                     | 91     | 4.0                                     | 102         |

(c) The exhalation resistance shall not exceed 25 mm. (1 inch) of water-column height at a flow rate of 85 liters (3 cubic feet) per minute when the blower is not operating or under any practical condition of blower operation.

**§ 11.124-11 Airflow resistance test, Type B and Type BE supplied-air respirators; minimum requirements.**

(a) Airflow resistance shall be determined when the respirator is completely assembled with the respiratory-inlet covering and the hose in the maximum length to be considered for approval, coiled in loops 1.5 to 2.1 m. (5 to 7 feet) in diameter.

(b) Airflow resistance shall not exceed 38 mm. (1.5 inches) of water-column height to air drawn at the flow rate of 85 liters (3 cubic feet) per minute.

(c) The exhalation resistance shall not exceed 25 mm. (1 inch) of water-column height at this flow rate.

**§ 11.124-12 Airflow resistance test, Type C supplied-air respirator, continuous flow class, and Type CE supplied-air respirator; minimum requirements.**

The resistance to air flowing from the respirator shall not exceed 25 mm. (1 inch) of water-column height when the air flow into the respiratory-inlet covering is 115 liters (4 cubic feet) per minute.

**§ 11.124-13 Airflow resistance test, Type C supplied-air respirator, demand class; minimum requirements.**

(a) Inhalation resistance shall not exceed 50 millimeters (2 inches) of water at an air flow of 115 liters (4 cubic feet) per minute.

(b) The exhalation resistance to a flow of air at a rate of 85 liters (3 cubic feet) per minute shall not exceed 25 millimeters (1 inch) of water.

**§ 11.124-14 Airflow resistance test, Type C supplied-air respirator, pressure-demand class; minimum requirements.**

(a) The static pressure in the facepiece shall not exceed 38 mm. (1.5 inches) of water-column height.

(b) The pressure in the facepiece shall not fall below atmospheric at inhalation airflows less than 115 liters (4 cubic feet) per minute.

(c) The exhalation resistance to a flow of air at a rate of 85 liters (3 cubic feet) per minute shall not exceed the static pressure in the facepiece by more than 51 mm. (2 inches) of water-column height.

**§ 11.124-15 Exhalation valve leakage test.**

(a) Dry exhalation valves and valve seats will be subjected to a suction of 25 mm. water-column height while in a normal operating position.

(b) Leakage between the valve and valve seat shall not exceed 30 milliliters per minute.

**§ 11.124-16 Man tests for gases and vapors; supplied-air respirators; general performance requirements.**

(a) Wearers will enter a chamber containing a gas or vapor as prescribed in §§ 11.124-17, 11.124-18, 11.124-19, and 11.124-20.

(b) Each wearer will spend 10 minutes in work to provide observations on freedom of the device from leakage. The freedom and comfort allowed the wearer will also be considered.

(c) Time during the test period will be divided as follows:

(1) *Five minutes.* Walking, turning head, dipping chin; and

(2) *Five minutes.* Pumping air with a tire pump into a 28-liter (1 cubic foot) container, or equivalent work.

(d) No odor of the test gas or vapor shall be detected by the wearer in the air breathed during any such test, and the wearer shall not be subjected to any undue discomfort or encumbrance because of the fit, air delivery, or other features of the respirator during the testing period.

§ 11.124-17 Man test for gases and vapors; Type A and Type AE respirators; test requirements.

(a) The completely assembled respirator will be worn in a chamber containing  $0.1 \pm 0.025$  percent isoamyl acetate vapor, and the intake of the hose, and not more than 25 percent of the hose length will be located in isoamyl acetate-free air.

(b) The man in the isoamyl acetate atmosphere will draw his inspired air through the hose, connections, and all parts of the air device by means of his lungs alone (blower not operating).

(c) The 10-minute work test will be repeated with the blower in operation at any practical speed up to 50 revolutions of the crank per minute.

§ 11.124-18 Man test for gases and vapors; Type B and Type BE respirators; test requirements.

(a) The completely assembled respirator will be worn in a chamber containing  $0.1 \pm 0.025$  percent isoamyl acetate vapor, and the intake of the hose, and not more than 25 percent of the hose length will be located in isoamyl acetate-free air.

(b) The man in the isoamyl acetate atmosphere will draw his inspired air through the hose and connections by means of his lungs alone.

§ 11.124-19 Man test for gases and vapors; Type C respirators, continuous-flow class and Type CE supplied-air respirators; test requirements.

(a) The completely assembled respirator will be worn in a chamber containing  $0.1 \pm 0.025$  percent isoamyl acetate vapor, the intake of the hose will be connected to a suitable source of respirable air, and not more than 25 percent of the hose length will be located in isoamyl acetate-free air.

(b) The minimum flow of air required to maintain a positive pressure in the respiratory-inlet covering throughout the entire breathing cycle will be supplied to the wearer, provided however, that airflow shall not be less than 115 liters per minute for tight-fitting and not less than 170 liters per minute for loose-fitting respiratory inlet-coverings.

(c) The test will be repeated with the maximum rate of flow attainable within specified operating pressures.

§ 11.124-20 Man test for gases and vapors; Type C supplied-air respirators, demand and pressure-demand classes; test requirements.

(a) The completely assembled respirator will be worn in a chamber containing  $0.1 \pm 0.025$  percent isoamyl acetate vapor, the intake of the hose will be connected to a suitable source of respirable air, and not more than 25 percent of the hose length will be located in isoamyl acetate-free air.

(b) The test will be conducted at the minimum pressure with the maximum hose length and will be repeated at the

maximum pressure with the minimum hose length.

§ 11.124-21 Tests for protection during abrasive blasting; Type AE, Type BE, and Type CE supplied-air respirators; general performance requirements.

(a) Tests will be made under conditions of typical abrasive blasting operation.

(b) The tests prescribed in §§ 11.124-22, 11.124-23, and 11.124-24 will be conducted under the following conditions:

(1) A suction-feed abrasive blasting outfit will be used by the wearer;

(2) The diameter of the air jet shall be 5 mm. ( $\frac{3}{16}$  inch);

(3) Air pressure will be 276-483 kN/m<sup>2</sup> (40-70 pounds per square inch);

(4) The abrasive used will contain a composition of 99+ percent free silica (SiO<sub>2</sub>);

(5) The size properties of the abrasive used will be a mixture of 90 percent by weight of essentially No. 1 sandblast sand and 10 percent air-floated fines; and

(6) The No. 1 sand used will meet a size specification of not more than 10 percent on a 20-mesh sieve and not more than 10 percent through a 35-mesh sieve; 99+ percent of the fines will be able to pass through a 270-mesh sieve. All size determinations will be made by standard-mesh sieves.

(c) Tests will be conducted for 30 minutes continuously.

(d) (1) The person wearing the respirator will sandblast the inside surface of a common iron kettle of approximate hemispherical shape (about 76 cm. (30 inches) in diameter, and 113.6 liters (30 gallons) capacity).

(2) The kettle will be placed with the plane of the opening inclined 45° from a vertical position and with the lowest point of the rim at about the height of the person's hips.

(3) The wearer will stand at one position in front of the kettle and lean over until the upper part of the body is inclined to parallel the face of the kettle.

(4) The wearer will blast the entire inner surface of the kettle with the blast at all times directed approximately at right angles to the surface with the nozzle of the gun approximately 15 cm. (6 inches) from the surface, and with his head approximately 46 cm. (18 inches) from the nozzle.

(5) The wearer will move his head forward, backward, and sideways during each blasting operation.

(e) (1) Air will be withdrawn continuously during the test at the rate of 32 liters (1.13 cubic feet) per minute from the respiratory-inlet covering at a point as near as convenient to the wearer's nostrils.

(2) Simultaneously air will be drawn at the same rate from the source of intake air to the respirator.

(f) Respirators tested in accordance with §§ 11.124-22, 11.124-23, and 11.124-24 shall meet the following minimum requirements:

(1) The amount of particulate matter in the air withdrawn from the respiratory-inlet covering shall not exceed the amount of particulate matter supplied to the respirator by more than 0.5 mg. for the 30-minute test period;

(2) The wearer of the respirator in this test shall not experience undue encumbrance and discomfort because of the fit, air delivery, or other features of the respirator; and,

(3) The head and shoulder covering shall adequately protect the wearer from discomfort or injury due to impact or abrasion from the rebounding material during the test.

§ 11.124-22 Test for protection during abrasive blasting; Type AE supplied-air respirator; test requirements.

(a) The respirator will be arranged as prescribed in § 11.124-17(a), and the tests prescribed in § 11.124-21 will be performed.

(b) The wearer will draw his inspired air through the hose, connections, and all parts of the air device by means of his lungs alone (blower not operating).

(c) The test will be repeated with the blower in operation at any practical speed up to 50 revolutions per minute of the crank.

§ 11.124-23 Test for protection during abrasive blasting; Type BE supplied-air respirator; test requirements.

(a) The respirator will be arranged as prescribed in § 11.124-18(a), and the tests prescribed in § 11.124-21 will be performed.

(b) The wearer will draw his inspired air through the hose, connections, and all parts of the air device by means of his lungs alone.

§ 11.124-24 Test for protection during abrasive blasting; Type CE supplied-air respirator; test requirements.

(a) The respirator will be arranged as prescribed in § 11.124-19(a), and the tests prescribed in § 11.124-21 will be performed.

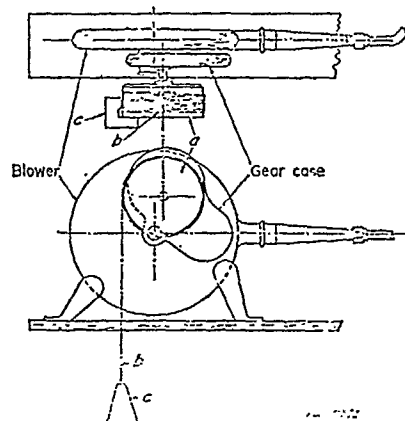


Figure 1.—Apparatus for measuring power required to operate blower. (39 CFR Part 11, Subpart J, § 11.124-3)



**Subpart K—Dust, Fume, and Mist Respirators**

**§ 11.130 Dust, fume, and mist respirators; description.**

Dust, fume, and mist respirators, including all completely assembled respirators designed for use as respiratory protection during entry into and escape from hazardous particulate atmospheres which contain adequate oxygen to support life, are described as follows:

(a) Respirators, either with replaceable or reusable filters, designed as respiratory protection against dusts (1) having an air contamination level not less than 0.05 milligram per cubic meter of air, including but not limited to coal, arsenic, cadmium, chromium, lead, and manganese; or (2) dusts having an air contamination level not less than 2 million particles per cubic foot of air, including but not limited to aluminum, flour, iron ore, and free silica, resulting principally from the disintegration of a solid, e.g., dust clouds produced in mining, quarrying, and tunneling, and in dusts produced during industrial operations, such as grinding, crushing, and the general processing of minerals and other materials.

(b) Respirators, with replaceable filters, designed as respiratory protection against fumes of various metals having an air contamination level not less than 0.05 milligram per cubic meter, including but not limited to aluminum, antimony, arsenic, cadmium, chromium, copper, iron, lead, magnesium, manganese, mercury (except mercury vapor), and zinc, which result from the sublimation or condensation of their respective vapors, or from the chemical reaction between their respective vapors and gases.

(c) Respirators, with replaceable filters, designed as respiratory protection against mists of materials having an air contamination level not less than 0.05 milligram per cubic meter or 2 million particles per cubic foot, e.g., mists produced by spray coating with vitreous enamels, chromic acid mist produced during chromium plating, and other mists of materials whose liquid vehicle does not produce harmful gases or vapors.

(d) Respirators, with replaceable filters, designed as respiratory protection against dusts, fumes, and mists having an air contamination level less than 0.05 milligram per cubic meter, including but not limited to lithium hydride and beryllium, and against radionuclides.

(e) Respirators, with replaceable filters, designed as respiratory protection against radon daughters, and radon daughters attached to dusts, fumes, and mists.

(f) Respirators, with replaceable filters, designed as respiratory protection against asbestos-containing dusts and mists.

(g) Respirators, with replaceable filters, designed as protection against various combinations of particulate matter.

(h) Single-use dust respirators designed as respiratory protection against pneumoconiosis- and fibrosis-producing

dusts, or dusts and mists, including but not limited to aluminum, asbestos, coal, flour, iron ore, and free silica.

(i) The types of dust, fume, and mist respirators in paragraphs (a) through (g) of this section may also be classified according to their design as follows:

- (1) Air-purifying respirators; and
- (2) Powered air-purifying respirators.

**§ 11.131 Dust, fume and mist respirators; required components.**

(a) Each dust, fume, and mist respirator described in § 11.130 shall, where its design requires, contain the following component parts:

- (1) Facepiece, mouthpiece with noseclip, hood, or helmet;
- (2) Filter unit;
- (3) Harness;
- (4) Attached blower; and
- (5) Breathing tube.

(b) The components of each dust, fume, and mist respirator shall meet the minimum construction requirements set forth in Subpart G of this part.

**§ 11.132 Breathing tubes; minimum requirements.**

(a) Flexible breathing tubes used in conjunction with respirators shall be designed and constructed to prevent:

- (1) Restriction of free head movement;
- (2) Disturbance of the fit of facepieces, mouthpieces, hoods, or helmets;
- (3) Interference with the wearer's activities; and
- (4) Shutoff of airflow due to kinking, or from chin or arm pressure.

**§ 11.133 Harnesses; installation and construction; minimum requirements.**

(a) Each respirator shall, where necessary, be equipped with a suitable harness designed and constructed to hold the components of the respirator in position against the wearer's body.

(b) Harnesses shall be designed and constructed to permit easy removal and replacement of respirator parts, and, where applicable, provide for holding a full facepiece in the ready position when not in use.

**§ 11.134 Respirator containers; minimum requirements.**

(a) Except as provided in paragraph (b) of this section each respirator shall be equipped with a substantial, durable container bearing markings which show the applicant's name, the type of respirator it contains, and all appropriate approval labels.

(b) Containers for single-use respirators may provide for storage of more than one respirator, however, such containers shall be designed and constructed to prevent contamination of respirators which are not removed, and to prevent damage to respirators during transit.

**§ 11.135 Half-mask facepieces, full facepieces, hoods, helmets, and mouthpieces; fit; minimum requirements.**

(a) Half-mask facepieces and full facepieces shall be designed and con-

structed to fit persons with various facial shapes and sizes either: (1) By providing more than one facepiece size, or (2) by providing one facepiece size which will fit varying facial shapes and sizes.

(b) Full facepieces shall provide for optional use of corrective spectacles or lenses, which shall not reduce the respiratory protective qualities of the respirator.

(c) Hoods and helmets shall be designed and constructed to fit persons with various head sizes, provide for the optional use of corrective spectacles or lenses, and insure against any restriction of movement by the wearer.

(d) Mouthpieces shall be equipped with noseclips which are securely attached to the mouthpiece or respirator and provide an airtight seal.

(e) Facepieces, hoods, and helmets shall be designed to prevent eyepiece fogging.

(f) Half-mask facepieces shall not interfere with the fit of common industrial safety corrective spectacles, as determined by the Bureau's facepiece tests in §§ 11.140-1 and 11.140-2.

**§ 11.136 Facepieces, hoods, and helmets; eyepieces; minimum requirements.**

Facepieces, hoods, and helmets shall be designed and constructed to provide adequate vision which is not distorted by the eyepieces.

**§ 11.137 Inhalation and exhalation valves; minimum requirements.**

(a) Inhalation and exhalation valves shall be protected against distortion.

(b) Inhalation valves shall be designed and constructed and provided where necessary to prevent excessive exhaled air from adversely affecting filters, except where filters are specifically designed to resist moisture as prescribed in § 11.140-5.

(c) Exhalation valves shall be: (1) Provided where necessary; (2) protected against damage and external influence; and (3) designed and constructed to prevent inward leakage of contaminated air.

**§ 11.138 Head harnesses; minimum requirements.**

(a) All facepieces shall be equipped with head harnesses designed and constructed to provide adequate tension during use and an even distribution of pressure over the entire area in contact with the face.

(b) Facepiece head harnesses, except those employed on single-use respirators, shall be adjustable and replaceable.

(c) Mouthpieces shall be equipped, where applicable, with adjustable and replaceable harnesses, designed and constructed to hold the mouthpiece in place.

**§ 11.139 Air velocity and noise levels; hoods and helmets; minimum requirements.**

Noise levels generated by the respirator will be measured inside the hood or helmet at maximum airflow obtainable and shall not exceed 80 dBA.

## RULES AND REGULATIONS

## § 11.140 Dust, fume, and mist respirators; performance requirements; general.

Dust, fume, and mist respirators and the individual components of each such device shall, as appropriate, meet the requirements for performance and protection specified in the tests described in §§ 11.140-1 through 11.140-12 and prescribed in Tables 9 and 10.

## § 11.140-1 Isoamyl acetate tightness test; dust, fume, and mist respirators designed for respiratory protection against fumes of various metals having an air contamination level not less than 0.05 milligram per cubic meter; minimum requirements.

(a) The respirator will be modified in such a manner that all of the air that normally would be inhaled through the inhalation port(s) is drawn through an efficient activated charcoal-filled canister, or cartridge(s), without interference with the face-contacting portion of the facepiece.

(b) The modified respirator will be worn by persons for at least 2 minutes each in a test chamber containing 100 parts (by volume) of isoamyl-acetate vapor per million parts of air.

(c) The odor of isoamyl-acetate shall not be detected by the wearers of the modified respirator while in the test atmosphere.

## § 11.140-2 Isoamyl acetate tightness test; respirators designed for respiratory protection against dusts, fumes, and mists having an air contamination level less than 0.05 milligram per cubic meter, or against radionuclides; minimum requirements.

(a) The applicant shall provide a charcoal-filled canister or cartridge of a size and resistance similar to the filter unit with connectors which can be attached to the facepiece in the same manner as the filter unit.

(b) (1) The canister or cartridge will be used in place of the filter unit, and persons will each wear a modified half-mask facepiece for 5 minutes in a test chamber containing 100 parts (by volume) of isoamyl-acetate vapor per million parts of air.

(2) The following work schedule will be performed by each wearer in the test chamber:

(i) Two minutes walking, nodding, and shaking head in normal movements; and

(ii) Three minutes exercising and running in place.

(3) The facepiece shall be capable of adjustment, according to the applicant's instructions, to each wearer's face, and the odor of isoamyl-acetate shall not be detected by any wearer during the test.

(c) When the respirator is equipped with a full facepiece, hood, helmet, or mouthpiece, the canister or cartridge will be used in place of the filter unit, and persons will each wear the modified respiratory unit covering for 5 minutes in a test chamber containing 1,000 parts (by volume) of isoamyl-acetate vapor per million parts of air, performing the work

schedule specified in paragraph (b) (2) of this section.

## § 11.140-3 Air-purifying filter tests; performance requirements; general.

Dust, fume, and mist respirators will be tested in accordance with the schedule set forth in Table 10 to determine their effectiveness as protection against the particulate hazards specified therein.

## § 11.140-4 Silica dust test; single-use or reusable filters; minimum requirements.

(a) Three respirators with single-use filters will be tested for periods of 90 minutes each at a continuous airflow rate of 32 liters per minute for air-purifying respirators, and for periods of 4 hours each at a flowrate not less than 115 liters per minute to tight-fitting facepieces, and not less than 170 liters per minute to loose-fitting hoods and helmets for powered air-purifying respirators.

(b) The relative humidity in the test chamber will be 20-80 percent, and the room temperature approximately 25° C.

(c) The test suspension in the chamber will not be less than 50 nor more than 60 milligrams of flint (99+ percent free silica) per cubic meter of air.

(d) The flint in suspension will be ground to pass 99+ percent through a 270-mesh sieve.

(e) The particle-size distribution of the test suspension will have a geometric mean of 0.4 to 0.6 micrometer, and the standard geometric deviation will not exceed 2.

(f) The total amount of unretained test suspension in samples taken during testing shall not exceed 1.5 milligrams for an air-purifying respirator, 14.4 milligrams for a powered air-purifying respirator with tight-fitting facepiece, and 21.3 milligrams for a powered air-purifying respirator with loose-fitting hood or helmet.

(g) Three respirators with reusable filters will be tested and shall meet the requirements specified in paragraphs (a) through (f) of this section; each filter shall be tested three times: Once as received; once after cleaning; and once after recleaning. The applicant's instructions shall be followed for each cleaning.

## § 11.140-5 Silica-dust test; single-use dust respirators; minimum requirements.

(a) Three respirators will be tested.

(b) As described in § 11.140-4, airflow will be cycled through the respirator by a breathing machine at the rate of 24 respirations per minute with a minute volume of 40 liters; a breathing machine cam with a work rate of 622 kg.-m.<sup>2</sup>/minute shall be used.

(c) Air exhaled through the respirator will be 35° ± 2° C. (95° ± 3° F.) with 94 ± 3 percent relative humidity.

(d) Air inhaled through the respirator will be sampled and analyzed for respirator leakage.

(e) The total amount of unretained test suspension, after drying, in samples

taken during testing, shall not exceed 1.8 milligrams for any single test.

## § 11.140-6 Lead fume test; minimum requirements.

(a) Three respirators will be tested for a period of 312 minutes each at a continuous airflow rate of 32 liters per minute for air-purifying respirators, and for periods of 4 hours each at a flow rate not less than 115 liters per minute to tight-fitting facepieces, and not less than 170 liters per minute to loose-fitting hoods and helmets for powered air-purifying respirators.

(b) The relative humidity in the test chamber will be 20-80 percent, and the room temperature approximately 25° C.

(c) The test suspension in the test chamber will not be less than 15 nor more than 20 milligrams of freshly generated lead-oxide fume, calculated as lead (Pb), per cubic meter of air.

(d) The fume will be generated by impinging an oxygen-gas flame on molten lead.

(e) Samples of the test suspension will be taken during each test period for analysis.

(f) The total amount of unretained test suspension in the samples taken during testing, which is analyzed and calculated as lead (Pb), shall not exceed 1.5 milligrams of lead for an air-purifying respirator, 4.2 milligrams of lead for a powered air-purifying respirator with tight-fitting facepiece, and 6.2 milligrams of lead for a powered air-purifying respirator with loose-fitting hood or helmet.

## § 11.140-7 Silica mist test; minimum requirements.

(a) Three respirators will be tested for a period of 312 minutes each at a continuous airflow rate of 32 liters per minute for air-purifying respirators, and for periods of 4 hours each at a flow rate not less than 115 liters per minute to tight-fitting facepieces, and not less than 170 liters per minute to loose-fitting hoods and helmets for powered air-purifying respirators.

(b) The room temperature in the test chamber will be approximately 25° C.

(c) The test suspension in the test chamber will not be less than 20 nor more than 25 milligrams of silica mist, weighed as silica dust, per cubic meter of air.

(d) Mist will be produced by spraying an aqueous suspension of flint (99+ percent free silica), and the flint shall be ground to pass 99+ percent through a 270-mesh sieve.

(e) Samples of the test suspension will be taken during each test period for analysis.

(f) The total amount of silica mist unretained in the samples taken during testing, weighed as silica dust, shall not exceed 2.5 milligrams for an air-purifying respirator, 6.9 milligrams for a powered air-purifying respirator with tight-fitting facepiece, and 10.2 milligrams for a powered air-purifying respirator with loose-fitting hood or helmet.

§ 11.140-8 Tests for respirators designed for respiratory protection against more than one type of dispersoid; minimum requirements.

Respirators designed as respiratory protection against more than one particulate hazard (dust, fume, or mist) shall comply with all the requirements of this part, with respect to each of the specific hazards involved.

§ 11.140-9 Airflow resistance tests; all dust, fume, and mist respirators; minimum requirements.

(a) Resistance to airflow will be measured in the facepiece, mouthpiece, hood, or helmet of a dust, fume, or mist respirator mounted on a test fixture with air flowing at a continuous rate of 85 liters per minute, both before and after each test conducted in accordance with §§ 11.140-4 through 11.140-7.

(b) The maximum allowable resistance requirements for dust, fume, and mist respirators are as follows:

| Type of respirator                                | MAXIMUM RESISTANCE<br>(mm. water-column height) |                  |            |
|---------------------------------------------------|-------------------------------------------------|------------------|------------|
|                                                   | Initial Inhalation                              | Final Inhalation | Exhalation |
| Single-use.....                                   | 12                                              | 15               | 15         |
| Dust, fume, and mist, with single-use filter..... | 30                                              | 60               | 20         |
| Dust, fume, and mist, with reusable filter.....   | 20                                              | 40               | 20         |
| Radon daughter.....                               | 18                                              | 25               | 15         |
| Asbestos dust and mist.....                       | 18                                              | 25               | 15         |

<sup>1</sup> Measured after silica dust test described in § 11.140-4.

§ 11.140-10 Exhalation valve leakage test; minimum requirements.

(a) Dry exhalation valves and valve seats will be subjected to a suction of 25 mm. water-column height while in a normal operating position.

(b) Leakage between the valve and valve seat shall not exceed 30 milliliters per minute.

TABLE 10—AIR-PURIFYING AND POWERED AIR-PURIFYING RESPIRATOR FILTER TESTS REQUIRED FOR APPROVAL  
(30 CFR Part 11, Subpart K, § 11.140-4, et seq.)

| Respirator types                                                                                                         | Silica dust tests |                |           | Lead fume test | Silica mist test | DOP test  |
|--------------------------------------------------------------------------------------------------------------------------|-------------------|----------------|-----------|----------------|------------------|-----------|
|                                                                                                                          | 11.140-4          | 11.140-5       | 11.140-12 | 11.140-6       | 11.140-7         | 11.140-11 |
| Dusts: Air Contamination Level not less than 0.05 mg/M <sup>3</sup> or 2 mppcf.....                                      | X                 |                |           |                |                  |           |
| Fumes: Air Contamination Level not less than 0.05 mg/M <sup>3</sup> .....                                                |                   |                |           | X              |                  |           |
| Mists: Air Contamination Level not less than 0.05 mg/M <sup>3</sup> .....                                                |                   |                |           |                | X                |           |
| Dusts, Fumes, and Mists: Air Contamination Level not less than 0.05 mg/M <sup>3</sup> or 2 mppcf, and radionuclides..... |                   |                | X         |                |                  | X         |
| Radon daughters.....                                                                                                     | X <sup>1</sup>    |                |           | X <sup>1</sup> |                  |           |
| Asbestos-containing dusts and mists.....                                                                                 | X <sup>1</sup>    |                |           |                | X <sup>1</sup>   |           |
| Single-use dust and mist respirators.....                                                                                |                   | X <sup>1</sup> |           |                | X <sup>1</sup>   |           |

<sup>1</sup> For resistance only.

<sup>2</sup> For penetration only.

<sup>3</sup> Test required only where applicable.

§ 11.140-11 DOP filter test: respirators designed as respiratory protection against dusts, fumes, and mists having an air contamination level less than 0.05 milligram per cubic meter and against radionuclides; minimum requirements.

(a) All single air-purifying respirator filter units will be tested in an atmosphere concentration of 100 micrograms of DOP per liter of air at continuous flow rates of 32 and 85 liters per minute for a period of 5 to 10 seconds.

(b) Where filters are to be used in pairs, the flow rates will be 16 and 42.5 liters per minute, respectively, through each filter.

(c) The filter will be mounted on a connector in the same manner as used on the respirator, and the total leakage for the connector and filter shall not exceed 0.03 percent of the ambient DOP concentration at either flow rate.

§ 11.140-12 Silica dust loading test; respirators designed as protection against dusts, fumes, and mists having an air contamination level less than 0.05 milligram per cubic meter and against radionuclides; minimum requirements.

Three respirators will be tested in accordance with the provisions of § 11.140-4 and shall meet the minimum requirements of §§ 11.140-4 and 11.140.9.

TABLE 9.—FACEPIECE TEST REQUIREMENTS  
(30 CFR Part 11, Subpart K, § 11.140-1, et seq.)

| Respirator types                                                                                                         | Pressure tightness test <sup>1</sup> | Isocamp acetate test |          |
|--------------------------------------------------------------------------------------------------------------------------|--------------------------------------|----------------------|----------|
|                                                                                                                          |                                      | 11.140-1             | 11.140-2 |
| Dusts: Air Contamination Level not less than 0.05 mg/M <sup>3</sup> or 2 mppcf.....                                      | X                                    |                      |          |
| Fumes: Air Contamination Level not less than 0.05 mg/M <sup>3</sup> .....                                                | X                                    | X                    |          |
| Mists: Air Contamination Level not less than 0.05 mg/M <sup>3</sup> or 2 mppcf.....                                      | X                                    |                      |          |
| Dusts, Fumes, and Mists: Air Contamination Level not less than 0.05 mg/M <sup>3</sup> or 2 mppcf, and radionuclides..... | X                                    |                      | X        |
| Radon daughters.....                                                                                                     | X                                    | X                    |          |
| Asbestos-containing dusts and mists.....                                                                                 | X                                    |                      |          |

<sup>1</sup> Test is required only where applicable.

#### Subpart L—Chemical Cartridge Respirators

§ 11.150 Chemical cartridge respirators; description.

Chemical cartridge respirators including all completely assembled respirators which are designed for use as respiratory protection during entry into or escape from atmospheres not immediately dangerous to life and health, are described according to the specific gases or vapors against which they are designed to provide respiratory protection, as follows:

| Type of chemical cartridge respirator: | Maximum use concentration, parts per million |
|----------------------------------------|----------------------------------------------|
| Ammonia .....                          | 300                                          |
| Chlorine .....                         | 10                                           |
| Hydrogen chloride.....                 | 50                                           |
| Methyl amine.....                      | 100                                          |
| Organic vapor <sup>1</sup> .....       | *1,000                                       |
| Sulfur dioxide.....                    | 50                                           |

<sup>1</sup> Not for use against organic vapors with poor warning properties or those which generate high heats of reaction with sorbent material in the cartridge.

\* Maximum use concentrations are lower for organic vapors which produce atmospheres immediately hazardous to life or health at concentrations equal to or lower than this concentration.

NOTE: Chemical cartridge respirators for respiratory protection against gases or vapors, which are not specifically listed with their maximum use concentration except pesticides, may be approved if the applicant submits a request for such approval, in writing, to the Bureau. The Bureau and the Institute shall consider each such application and accept or reject the application after a review of the effects on the wearer's health and safety and in the light of any field experience in use of chemical cartridge respirators as protection against such hazards.

§ 11.151 Chemical cartridge respirators; required components.

(a) Each chemical cartridge respirator described in § 11.150 shall, where its design requires, contain the following component parts:

- (1) Facepiece, mouthpiece, and nose-clip, hood, or helmet;
- (2) Cartridge;
- (3) Cartridge with filter;
- (4) Harness;
- (5) Breathing tube; and
- (6) Attached blower.

(b) The components of each chemical cartridge respirator shall meet the minimum construction requirements set forth in Subpart G of this part.

§ 11.152 Cartridges in parallel; resistance requirements.

Where two or more cartridges are used in parallel, their resistance to airflow shall be essentially equal.

§ 11.153 Cartridges: color and markings; requirements.

The color and markings of all cartridges or labels shall conform with the requirements of the American National Standard for Identification of Gas Mask

## RULES AND REGULATIONS

Canisters, K13.1, obtainable from American National Standards Institute, Inc., 1430 Broadway, New York, NY 10018.

**§ 11.154 Filters used with chemical cartridges; location; replacement**

(a) Particulate matter filters used in conjunction with a chemical cartridge shall be located on the inlet side of the cartridge.

(b) Filters shall be incorporated in or firmly attached to the cartridge and each filter assembly shall, where applicable, be designed to permit its easy removal from and replacement on the cartridge.

**§ 11.155 Breathing tubes; minimum requirements.**

(a) Flexible breathing tubes used in conjunction with respirators shall be designed and constructed to prevent:

- (1) Restriction of free head movement;
- (2) Disturbance of the fit of facepieces, mouthpieces, hoods, or helmets;
- (3) Interference with the wearer's activities; and
- (4) Shutoff of airflow due to kinking, or from chin or arm pressure.

**§ 11.156 Harnesses; installation and construction; minimum requirements.**

(a) Each respirator shall, where necessary, be equipped with a suitable harness designed and constructed to hold the components of the respirator in position against the wearer's body.

(b) Harnesses shall be designed and constructed to permit easy removal and replacement of respirator parts and, where applicable, provide for holding a full facepiece in the ready position when not in use.

**§ 11.157 Respirator containers; minimum requirements.**

Respirators shall be equipped with a substantial, durable container bearing markings which show the applicant's name, the type and commercial designation of the respirator it contains and all appropriate approval labels.

**§ 11.158 Half-mask facepieces, full facepieces, mouthpieces, hoods, and helmets; fit; minimum requirements.**

(a) Half-mask facepieces and full facepieces shall be designed and constructed to fit persons with various facial shapes and sizes either: (1) By providing more than one facepiece size, or (2) by providing one facepiece size which will fit varying facial shapes and sizes.

(b) Hoods and helmets shall be designed and constructed to fit persons with various head sizes, provide for the optional use of corrective spectacles or lenses, and insure against any restriction of movement by the wearer.

(c) Mouthpieces shall be equipped with noseclips which are securely attached to the mouthpiece or respirator and provide an airtight fit.

(d) Full facepieces shall provide for optional use of corrective spectacles or lenses which shall not reduce the respiratory protective qualities of the respirator.

(e) Facepieces, hoods, and helmets shall be designed to prevent eyepiece fogging.

**§ 11.158-1 Facepieces, hoods, and helmets; eyepieces; minimum requirements.**

Facepieces, hoods, and helmets shall be designed and constructed to provide adequate vision which is not distorted by the eyepieces.

**§ 11.159 Inhalation and exhalation valves; minimum requirements.**

(a) Inhalation and exhalation valves shall be provided where necessary and protected against distortion.

(b) Inhalation valves shall be designed and constructed to prevent excessive exhaled air from entering cartridges or adversely affecting canisters.

(c) Exhalation valves shall be: (1) Protected against damage and external influence, and (2) designed and constructed to prevent inward leakage of contaminated air.

**§ 11.160 Head harnesses; minimum requirements.**

(a) Facepieces shall be equipped with adjustable and replaceable head harnesses designed and constructed to provide adequate tension during use and an even distribution of pressure over the entire area in contact with the face.

(b) Mouthpieces shall be equipped where applicable, with an adjustable and replaceable harness designed and constructed to hold the mouthpiece in place.

**§ 11.161 Air velocity and noise levels; hoods and helmets; minimum requirements.**

Noise levels generated by the respirator will be measured inside the hood or helmet at maximum airflow obtainable and shall not exceed 80 dBA.

**§ 11.162 Chemical cartridge respirators; performance requirements; general.**

Chemical cartridge respirators and the individual components of each such device shall, as appropriate, meet the minimum requirements for performance and protection specified in the tests described in §§ 11.162-1 through 11.162-8.

**§ 11.162-1 Breathing resistance test; minimum requirements.**

(a) Resistance to airflow will be measured in the facepiece, mouthpiece, hood, or helmet of a chemical cartridge respirator mounted on a test fixture with air flowing at a continuous rate of 85 liters per minute, both before and after each test conducted in accordance with §§ 11.162-5 through 11.162-8.

(b) The maximum allowable resistance requirements for chemical cartridge respirators are as follows:

| Type of chemical cartridge respirator                                                   | MAXIMUM RESISTANCE<br>(min. water-column height) |                    | Exhalation |
|-----------------------------------------------------------------------------------------|--------------------------------------------------|--------------------|------------|
|                                                                                         | Inhalation                                       | Final <sup>1</sup> |            |
| For gases, vapors, or gases and vapors.....                                             | 40                                               | 45                 | 20         |
| For gases, vapors, or gases and vapors, and dusts, fumes, and mists.....                | 50                                               | 70                 | 20         |
| For gases, vapors, or gases and vapors, and mists of paints, lacquers, and enamels..... | 50                                               | 70                 | 20         |

<sup>1</sup> Measured at end of service life specified in Table 11.

**§ 11.162-2 Exhalation valve leakage test; minimum requirements.**

(a) Dry exhalation valves and valve seats will be subjected to a suction of 25 mm. water-column height while in a normal operating position.

(b) Leakage between the valve and valve seat shall not exceed 30 milliliters per minute.

**§ 11.162-3 Facepiece test; minimum requirements.**

(a) The complete chemical cartridge respirator will be fitted to the faces of persons having varying facial shapes and sizes.

(b) Where the applicant specifies a facepiece size or sizes for the respirator together with the approximate measurement of faces they are designed to fit, the Bureau will provide test subjects to suit such facial measurements.

(c) Any chemical cartridge respirator part which must be removed to perform the facepiece or mouthpiece fit test shall be replaceable without special tools and without disturbing facepiece or mouthpiece fit.

(d) The facepiece or mouthpiece fit test using the positive or negative pressure recommended by the applicant and described in his instructions will be used before each test.

(e) (1) Each wearer will enter a chamber containing 100 p.p.m. isoamyl acetate vapor for half-mask facepieces, and 1,000 p.p.m. for full facepieces, mouthpieces, hoods, and helmets.

(2) The facepiece or mouthpiece may be adjusted, if necessary, in the test chamber before starting the test.

(3) Each wearer will remain in the chamber for 8 minutes while performing the following activities:

(i) Two minutes, nodding and turning head;

(ii) Two minutes, calisthenic arm movements;

(iii) Two minutes, running in place; and

(iv) Two minutes, pumping with a tire pump into a 28-liter (1 cubic-foot) container.

(4) Each wearer shall not detect the odor of isoamyl-acetate vapor during the test.

§ 11.162-4 Lacquer and enamel mist tests; respirators with filters; minimum requirements; general.

(a) Three respirators with cartridges containing or having attached to them, filters for protection against mists of paints, lacquers, and enamels shall be tested in accordance with the provisions of § 11.162-8.

(b) In addition to the test requirements set forth in paragraph (a) of this section, three such respirators will be tested against each aerosol in accordance with the provisions of §§ 11.162-5 and 11.162-6.

§ 11.162-5 Lacquer mist test; minimum requirements.

(a) Temperature in the test chamber will be approximately 25° C.

(b) Continuous airflow through the respirator will be 32 liters per minute for air-purifying respirators, and not less than 115 liters per minute to tight fitting facepieces and 170 liters per minute to loose-fitting hoods and helmets of powered air-purifying respirators.

(c) Airflow through the chamber will be 20-25 air changes per minute.

(d) The atomizer employed will be a No. 64-5 nozzle with setup 3, or equivalent, operating at 69 kN/m<sup>2</sup>. (10 pounds per square inch gage).

(e) The test aerosol will be prepared by atomizing a mixture of one volume of clear cellulose nitrate lacquer and one volume of lacquer thinner.

(f) The lacquer used will conform essentially to Federal Specification TT-L-31, October 7, 1953.

(g) The concentration of cellulose nitrate in the test aerosol will be 95-125 milligrams per cubic meter.

(h) The test aerosol will be drawn to each respirator for a total of 156 minutes for air-purifying respirators and 240 minutes for powered air-purifying respirators.

(i) The total amount of unretained mist in the samples taken during testing, weighed as cellulose nitrate, shall not exceed 5 milligrams for an air-purifying respirator, 28 milligrams for a powered air-purifying respirator with tight-fitting facepiece, and 41 milligrams for a powered air-purifying respirator with loose-fitting hood or helmet.

§ 11.162-6 Enamel mist test; minimum requirements.

(a) Temperature in the test chamber will be approximately 25° C.

(b) Continuous airflow through the respirator will be 32 liters per minute for air-purifying respirators, and not less than 115 liters per minute to tight-fitting facepieces and 170 liters per minute to loose-fitting hoods and helmets of powered air-purifying respirators.

(c) Airflow through the chamber will be 20-25 air changes per minute.

(d) The atomizer employed will be a No. 64 nozzle with setup 1A, or equivalent, operating at 69 kN/m<sup>2</sup>. (10 pounds per square inch gage).

(e) The test aerosol will be prepared by atomizing a mixture of 1 volume of white enamel and 1 volume of turpentine.

(f) The enamel used will conform essentially to Federal Specification TT-E-489b, May 12, 1953 (an enamel having a phthalic alkyd resin vehicle and a titanium dioxide pigment).

(g) The concentration of pigment in the test aerosol, weighed as ash, will be 95-125 milligrams per cubic meter.

(h) The test aerosol will be drawn to each respirator for a total of 156 minutes for air-purifying respirators and 240 minutes for power air-purifying respirators.

(i) The total amount of unretained mist in the samples taken during testing, weighed as ash, shall not exceed 1.5 milligrams for any air-purifying respirator, 8.3 milligrams for a powered air-purifying respirator with tight-fitting facepiece, and 12.3 milligrams for a powered air-purifying respirator with loose-fitting hood or helmet.

§ 11.162-7 Dust, fume, and mist tests; respirators with filters; minimum requirements; general.

(a) Three respirators with cartridges containing, or having attached to them, filters for protection against dusts, fumes, and mists, except the mists of paints, lacquers, and enamels, will be tested in accordance with the provisions of § 11.162-8.

(b) In addition to the test requirements set forth in paragraph (a) of this section, three such respirators will be tested, as appropriate, in accordance with the provisions of §§ 11.140-1 through 11.140-14. however, the maximum allowable resistance of complete dust, fume, and mist, and gas, vapor, or gas and vapor chemical cartridge res-

pirators shall not exceed the maximum allowable limits set forth in § 11.162-1.

§ 11.162-8 Bench tests; gas and vapor tests; minimum requirements; general.

(a) Bench tests will be made on an apparatus that allows the test atmosphere at 50 ±5 percent relative humidity and room temperature, approximately 25° C., to enter the cartridges continuously at predetermined concentrations and rates of flow, and that has means for determining the test life of the cartridges.

(b) Where two cartridges are used in parallel on a chemical cartridge respirator, the bench test will be performed with the cartridges arranged in parallel, and the test requirements will apply to the combination rather than to the individual cartridges.

(c) Three cartridges or pairs of cartridges will be removed from containers and tested as received from the applicant.

(d) Two cartridges or pairs of cartridges will be equilibrated at room temperature by passing 25 percent relative humidity air through them at the following flow rates (expressed in liters per minute (l.p.m.)) for 6 hours:

| Type of cartridge:                                           | Airflow rate, l.p.m. |
|--------------------------------------------------------------|----------------------|
| Air purifying.....                                           | 25                   |
| Powered air purifying with tight-fitting facepiece.....      | 115                  |
| Powered air purifying with loose-fitting hood or helmet..... | 170                  |

(e) Two cartridges or pairs of cartridges will be equilibrated by passing 85 percent relative humidity air through them at the flow rates stated in paragraph (d) of this section.

(f) All cartridges will be resealed, kept in an upright position, at room temperatures, and tested within 18 hours.

(g) Cartridges will be tested and shall meet the minimum requirements set forth in Table 11.

TABLE 11.—CARTRIDGE BENCH TESTS AND REQUIREMENTS  
(30 CFR Part 11, Subpart L, § 11.162-8)

| Cartridge              | Test condition    | Test atmosphere                 |                        | Flowrate (l.p.m.) | Number of tests | Pass- Minimum          |        |
|------------------------|-------------------|---------------------------------|------------------------|-------------------|-----------------|------------------------|--------|
|                        |                   | Gas or vapor                    | Concentration (p.p.m.) |                   |                 | tration life* (p.p.m.) | (min.) |
| Ammonia.....           | As received.....  | NH <sub>3</sub>                 | 1000                   | 64                | 3               | 50                     | 60     |
| Ammonia.....           | Equilibrated..... | NH <sub>3</sub>                 | 1000                   | 32                | 4               | 50                     | 50     |
| Chlorine.....          | As received.....  | Cl <sub>2</sub>                 | 500                    | 64                | 3               | 5                      | 35     |
| Chlorine.....          | Equilibrated..... | Cl <sub>2</sub>                 | 500                    | 32                | 4               | 5                      | 35     |
| Hydrogen chloride..... | As received.....  | HCl                             | 500                    | 64                | 3               | 5                      | 50     |
| Hydrogen chloride..... | Equilibrated..... | HCl                             | 500                    | 32                | 4               | 5                      | 50     |
| Methyl amine.....      | As received.....  | CH <sub>3</sub> NH <sub>2</sub> | 1000                   | 64                | 3               | 10                     | 25     |
| Methyl amine.....      | Equilibrated..... | CH <sub>3</sub> NH <sub>2</sub> | 1000                   | 32                | 4               | 10                     | 25     |
| Organic vapors.....    | As received.....  | CCl <sub>4</sub>                | 1000                   | 64                | 3               | 5                      | 50     |
| Organic vapors.....    | Equilibrated..... | CCl <sub>4</sub>                | 1000                   | 32                | 4               | 5                      | 50     |
| Sulfur dioxide.....    | As received.....  | SO <sub>2</sub>                 | 500                    | 64                | 3               | 5                      | 30     |
| Sulfur dioxide.....    | Equilibrated..... | SO <sub>2</sub>                 | 500                    | 32                | 4               | 5                      | 30     |

\* Minimum life will be determined at the indicated concentration.  
\* Where a respirator is designed for respiratory protection against more than one type of gas or vapor, as for use in ammonia and in chlorine, the minimum life shall be equal to the lowest life for each type of gas or vapor. Where a respirator is designed for respiratory protection against more than one gas of a type, as for use in chlorine and sulfur dioxide, the stated minimal life shall apply.

**Subpart M—Pesticide Respirators****§ 11.170 Pesticide respirators; description.**

Pesticide respirators, including all completely assembled respirators which are designed for use as respiratory protection during entry into and escape from atmospheres which contain pesticide hazards, are described according to their construction as follows:

- (a) Front-mounted or back-mounted gas masks;
- (b) Chin-style gas mask;
- (c) Chemical cartridge;
- (d) Air-purifying respirator with attached blower; and,
- (e) Other devices, including combination respirators.

**§ 11.171 Pesticide respirators; required components.**

(a) Each pesticide respirator described in § 11.170 shall, where its design requires, contain the following component parts:

- (1) Facepiece, mouthpiece, and noseclip, helmet, or hood;
- (2) Canister with filter;
- (3) Cartridge with filter;
- (4) Harness;
- (5) Attached blower; and,
- (6) Breathing tube.

(b) The components of each pesticide respirator shall meet the minimum construction requirements set forth in Subpart G of this part.

**§ 11.172 Canisters and cartridges in parallel; resistance requirements.**

Where two or more canisters or cartridges are used in parallel, their resistance to airflow shall be essentially equal.

**§ 11.173 Canisters and cartridges; color and markings; requirements.**

The color and markings of all canisters and cartridges or labels shall conform with the requirements of the American National Standard for Identification of Gas Mask Canisters, K13.1.

**§ 11.174 Filters used with canisters and cartridges; location; replacement.**

(a) Particulate matter filters used in conjunction with a canister or cartridge shall be located on the inlet side of the canister or cartridge.

(b) Filters shall be incorporated into or firmly attached to the canister or cartridge and each filter assembly shall, where applicable, be designed to permit its easy removal from and replacement on the canister or cartridge.

**§ 11.175 Breathing tubes; minimum requirements.**

(a) Flexible breathing tubes used in conjunction with respirators shall be designed and constructed to prevent:

- (1) Interruption of free head movement;
- (2) Disturbance of the fit of facepieces, mouthpieces, hoods, or helmets;
- (3) Interference with the wearer's activities; and,
- (4) Shutoff of airflow due to kinking, or from chin or arm pressure.

**§ 11.176 Harnesses; installation and construction; minimum requirements.**

(a) Each respirator shall, where necessary, be equipped with a suitable harness designed and constructed to hold the components of the respirator in position against the wearer's body.

(b) Harnesses shall be designed and constructed to permit easy removal and replacement of respirator parts, and, where applicable, provide for holding a full facepiece in the ready position when not in use.

**§ 11.177 Respirator containers; minimum requirements.**

(a) Respirators shall be equipped with a substantial, durable, container bearing markings which show the applicant's name, type, and commercial designation of the respirator it contains, and all appropriate approval labels.

(b) Containers for gas masks shall be designed and constructed to permit easy removal of the mask.

**§ 11.178 Half-mask facepieces, full facepieces, hoods and helmets, and mouthpieces; fit; minimum requirements.**

(a) Half-mask facepieces and full facepieces shall be designed and constructed to fit persons with various facial shapes and sizes either: (1) By providing more than one facepiece size, or (2) by providing one facepiece size which will fit varying facial shapes and sizes.

(b) Full facepieces shall provide for optional use of corrective spectacles or lenses, which shall not reduce the respiratory protective quality of the respirator.

(c) Hoods and helmets shall be designed and constructed to fit persons with various head sizes, permit optional use of corrective spectacles without reducing the respiratory protective qualities of the respirator, and insure against any restriction of movement by the wearer.

(d) Pesticide respirators with mouthpieces shall be equipped with noseclips which are securely attached to the mouthpiece or respirator and provide an airtight seal.

(e) Facepieces, hoods, and helmets shall be designed to prevent eyepiece fogging.

(f) Half-mask facepieces shall not interfere with the fit of common industrial safety corrective spectacles as determined by the facepiece tests in § 11.183-3.

**§ 11.179 Facepieces, hoods, and helmets; eyepieces; minimum requirements.**

(a) Facepieces, hoods, and helmets shall be designed and constructed to provide adequate vision which is not distorted by the eyepiece.

(b) All eyepieces of gas masks shall be designed and constructed to meet the impact and penetration requirements specified in Federal Specification, Mask, Air line: and Respirator, Air Filtering,

Industrial, GGG-M-125d, October 11, 1965.

**§ 11.180 Inhalation and exhalation valves; minimum requirements.**

(a) Inhalation and exhalation valves shall be protected against distortion.

(b) Inhalation valves shall be designed and constructed and provided where necessary to prevent excessive exhaled air from adversely affecting cartridges, canisters, and filters.

(c) Exhalation valves shall be:

- (1) Provided where necessary;
- (2) Protected against damage and external influence; and,
- (3) Designed and constructed to prevent inward leakage of contaminated air.

**§ 11.181 Head harnesses; minimum requirements.**

(a) Facepieces shall be equipped with adjustable and replaceable head harnesses designed and constructed to provide adequate tension during use and an even distribution of pressure over the entire area in contact with the face.

(b) Mouthpieces shall be equipped, where applicable, with adjustable and replaceable harnesses designed and constructed to hold the mouthpiece in place.

**§ 11.182 Air velocity and noise levels; hoods and helmets; minimum requirements.**

Noise levels generated by the respirator will be measured inside the hood or helmet at maximum obtainable airflow and shall not exceed 80 dBA.

**§ 11.183 Pesticide respirators; performance requirements; general.**

Pesticide respirators and the individual components of each such device shall, as appropriate, meet the requirements for performance and protection specified in the tests described in §§ 11.183-1 through 11.183-7.

**§ 11.183-1 Breathing resistance test; minimum requirements.**

(a) Airflow resistance will be measured in the facepiece, mouthpiece, hood, or helmet of a pesticide respirator mounted on a test fixture with air flowing at a continuous rate of 85 liters per minute, both before and after each test conducted in accordance with §§ 11.183-4 and 11.183-7.

(b) The maximum allowable resistance requirements for pesticide respirators are as follows:

MAXIMUM RESISTANCE  
(mm. water-column height)

| Type of Pesticide respirator    | Inhalation |                    | Exhalation |
|---------------------------------|------------|--------------------|------------|
|                                 | Initial    | Final <sup>1</sup> |            |
| Front- or back-mounted gas mask | 70         | 85                 | 50         |
| Chin-style gas mask             | 65         | 80                 | 50         |
| Powered air-purifying           | 100        | 120                | 50         |
| Chemical cartridge              | 50         | 70                 | 50         |

<sup>1</sup> Measured at end of the service life specified in Table 12.

<sup>2</sup> Resistance of filter(s), cartridge(s), and breathing tube(s) only with blower not operating.

§ 11.183-2 Exhalation valve leakage test; minimum requirements.

(a) Dry exhalation valves and valve seats will be subjected to a suction of 25 mm. water-column height while in a normal operating position.

(b) Leakage between the valve and valve seat shall not exceed 30 milliliters per minute.

§ 11.183-3 Facepiece test; minimum requirements.

(a) The complete pesticide respirator will be fitted to the faces of persons having varying facial shapes and sizes.

(b) Where the applicant specifies a facepiece size or sizes for his respirator together with the approximate measurements of faces they are designed to fit, the Bureau will provide test subjects to suit such facial measurements.

(c) Any pesticide respirator part which must be removed to perform the facepiece fit test shall be replaceable without special tools and without disturbing facepiece fit.

(d) The facepiece or mouthpiece fit test using positive or negative pressure recommended by the applicant and described in his instructions will be used during each test.

(e) (1) Each wearer will enter a chamber containing 1,000 p.p.m. isoamyl-acetate vapor for a respirator equipped with a full facepiece, mouthpiece, hood, or helmet and 100 p.p.m. isoamyl-acetate vapor for a respirator equipped with a half-mask facepiece.

(2) The facepiece, mouthpiece, hood, or helmet may be adjusted, if necessary, in the test chamber before starting the test.

(3) Each wearer will remain in the chamber while performing the following activities:

(i) Two minutes, nodding and turning head;

(ii) Two minutes, calisthenic arm movements;

(iii) Two minutes, running in place; and,

(iv) Two minutes, pumping with a tire pump into a 28-liter (1 cubic foot) container.

(4) Each wearer shall not detect the odor of isoamyl-acetate during the test.

§ 11.183-4 Silica dust test; minimum requirements.

Three completely assembled pesticide respirators will be tested with a mechanical-testing apparatus as follows:

(a) Temperature in the test chamber will be approximately 25° C.

(b) Continuous airflow through the respirator will be 32 liters per minute for front-mounted, back-mounted, and chin-style gas mask pesticide respirators and chemical cartridge pesticide respirators, and not less than 115 (4 cubic feet) liters per minute to tight-fitting facepieces and 170 liters (6 cubic feet) per minute to loose-fitting hoods and helmets of powered air-purifying respirators.

(c) The test aerosol will contain 50-60 milligrams of 99+ percent free silica per cubic meter of air.

(d) The particle size distribution of the test suspension will have a geometric mean diameter of 0.4 to 0.6 micrometer, with a standard geometric deviation less than 2.

(e) Front-mounted, back-mounted, and chin-style gas mask pesticide respirators and chemical cartridge pesticide respirators will be tested for 90 minutes and powered air-purifying respirators will be tested for 4 hours.

§ 11.183-5 Lead fume test; minimum requirements.

Three completely assembled pesticide respirators will be tested with a mechanical-testing apparatus as follows:

(a) Continuous airflow through the respirator will be 32 liters per minute for front-mounted, back-mounted, and chin-style gas mask pesticide respirators and chemical cartridge pesticide respirators and not less than 115 liters (4 cubic feet) per minute, for powered air-purifying respirators with tight-fitting facepieces, and not less than 170 liters (6 cubic feet) per minute for powered air-purifying respirators with loose-fitting hoods and helmets.

(b) The test aerosol will contain 15-20 milligrams of freshly generated lead-oxide fume, calculated as lead, per cubic meter of air.

(c) The fume will be generated by impinging an oxygen-gas flame on molten lead.

(d) Front-mounted, back-mounted, and chin-style gas mask pesticide respirators and chemical cartridge pesticide respirators will be tested for 90 minutes and powered air-purifying pesticide respirators will be tested for 4 hours.

(e) The total amount of unretained test suspension, which is analyzed and calculated as lead, shall not exceed: (1) 0.43 milligram for any 90-minute test; (2) 4.8 milligrams for any 4-hour test made at 115 liters (4 cubic feet) per minute; or (3) 6.2 milligrams for any 4-hour test made at 170 liters (6 cubic feet) per minute.

§ 11.183-6 Diocetyl-phthalate test; minimum requirements.

(a) All canisters submitted for use with front-mounted and back-mounted

gas mask pesticide respirators will be tested in an atmospheric concentration of 100 micrograms of diocetyl-phthalate per liter of air at continuous flow rates of 32 and 85 liters per minute for a test period of 5 to 10 seconds.

(b) The DOP leakage through the canister shall not exceed 0.03 percent of the ambient DOP concentration.

§ 11.183-7 Bench tests; minimum requirements.

(a) (1) Bench tests will be made on an apparatus that allows the test atmosphere at 50±5 percent relative humidity and at room temperature (25°±2.5° C.) to enter the canister or cartridge at predetermined concentrations and rates of flow, and that has a means for determining the test life of the canister or cartridge against carbon tetrachloride.

(2) Canisters and cartridges will be tested as they are used on each pesticide respirator, either singly or in pairs.

(3) Three canisters or cartridges or pairs of cartridges will be removed from containers and tested as received from the applicant.

(4) Two canisters, cartridges, or pairs of cartridges will be equilibrated at room temperature by passing 25 percent relative humidity air through them at the following flow rates (expressed as liters per minute (l.p.m.)) for 6 hours:

| Type of canister or cartridge                                | Airflow rate, l.p.m. |
|--------------------------------------------------------------|----------------------|
| Air-purifying canister.....                                  | 64                   |
| Air-purifying cartridge.....                                 | 25                   |
| Powered air-purifying with tight-fitting facepiece.....      | 115                  |
| Powered air-purifying with loose-fitting hood or helmet..... | 170                  |

(5) Two canisters, cartridges, or pairs of cartridges will be equilibrated at room temperature by passing 85 percent relative humidity air through them at the flow rates stated in subparagraph (4) of this paragraph for 6 hours.

(6) The equilibrated canisters or cartridges will be resealed, kept in an upright position at room temperature, and tested within 18 hours.

(b) Canisters and cartridges tested in accordance with the provisions of this section shall meet the requirements specified in Table 12.

TABLE 12.—CARBON TETRACHLORIDE BENCH TESTS AND REQUIREMENTS FOR CANISTERS AND CARTRIDGES  
(30 CFR Part 11, Subpart M, § 11.183-7)

| Type of pesticide respirator                                                       | Test concentrations, p.p.m. CCl <sub>4</sub> | Flow rate, l.p.m. | Number of tests | Minimum life, minutes <sup>1</sup> |
|------------------------------------------------------------------------------------|----------------------------------------------|-------------------|-----------------|------------------------------------|
| Chest-mounted or back-mounted gas mask (as received).....                          | 20,000                                       | 64                | 3               | 12                                 |
| Chest-mounted or back-mounted gas mask (equilibrated).....                         | 20,000                                       | 32                | 4               | 12                                 |
| Chin-style gas mask (as received).....                                             | 5,000                                        | 64                | 3               | 9                                  |
| Chin-style gas mask (equilibrated).....                                            | 5,000                                        | 32                | 4               | 9                                  |
| Chemical cartridge respirator (as received).....                                   | 1,000                                        | 64                | 3               | 50                                 |
| Chemical cartridge respirator (equilibrated).....                                  | 1,000                                        | 32                | 4               | 50                                 |
| Powered air-purifying respirator (tight-fitting facepiece, as received).....       | 1,000                                        | 115               | 3               | 5                                  |
| Powered air-purifying respirator (tight-fitting facepiece, equilibrated).....      | 1,000                                        | 115               | 4               | 2                                  |
| Powered air-purifying respirator (loose-fitting hood or helmet, as received).....  | 1,000                                        | 170               | 3               | 50                                 |
| Powered air-purifying respirator (loose-fitting hood or helmet, equilibrated)..... | 1,000                                        | 170               | 4               | 25                                 |

<sup>1</sup> Minimum life will be determined at 5 p.p.m. leakage.

<sup>2</sup> The flow rate shall be the effective flow rate of the device, but shall be not less than 115 l.p.m.

<sup>3</sup> The flow rate shall be the effective flow rate of the device, but shall be not less than 170 l.p.m.

[FR Doc. 72-4116 Filed 3-24-72; 8:45 am]