

SEMI-VOLATILES FILE Processed: 03-19-1995 18:02:39, sequence: 1
RAW DATA SAVED IN FILE 03-19-1995.D

***** INTERNAL STANDARD TABLE *****
***** 03-19-1995 18:02:39 Version 5.1 *****
* Sample Name: SEMI-VOLATILES-415011 Data File: G:\P102049 *
* Date: 03-19-1995 18:02:39 Method: M:SEMIDEE 03-18-1995 08:59:58 # 168*
* Interface: 4 Cycle#: 49 Operator DLD Channel#: 0 Vial#: N.A. *
* Starting Peak Width: 3 Threshold: 1 Area Threshold: 50 *

* Instrument Type: HP 5890 2 SEP COLUMN Column Type: DB-5 15M 1.5u film *
* Solvent Description: HE DB-1701 30M 0.25ID 0.25u # *
* Conditions: 60 1MIN-15/MIN FINAL TEMP FID. VARIOUS FOR ECD *
* Detector 0: FID Detector 1: ECD #0 40 *
* Misc. Information: INJECTOR A 4psi, B 15 psi *

Starting Delay: 0.00 Ending retention time: 10.00
Area reject: 100 One sample per 0.300 sec.
Amount injected: 1.00 Dilution factor: 1.00
Internal Standard Amount: 1
Sample Weight: 1.00000


PEAK NUM	RET TIME	PEAK NAME	CONCENTRATION in PPB	NORMALIZED CONC	AREA	AREA/ HEIGHT	HEIGHT BL	REF PEAK	INT. STD PEAK	% DELTA RET TIME	CONC/AREA
1	0.550		0.0000	0.0000Z	11425	446	25.6 1		24		0.0000E+00
2	0.750		0.0000	0.0000Z	284	155	1.8 1		24		0.0000E+00
3	0.815		0.0000	0.0000Z	828	644	1.3 1		24		0.0000E+00
4	0.865		0.0000	0.0000Z	181	148	1.2 1		24		0.0000E+00
5	0.915		0.0000	0.0000Z	1070	572	1.9 1		24		0.0000E+00
6	1.195		0.0000	0.0000Z	5108037	267453	19.1 1		24		0.0000E+00
7	2.005		0.0000	0.0000Z	516238	22234	23.2 1		24		0.0000E+00
8	2.065		0.0000	0.0000Z	80336	26968	3.0 1		24		0.0000E+00
9	2.170		0.0000	0.0000Z	3174245	316634	10.0 1		24		0.0000E+00
10	2.600		0.0000	0.0000Z	25840	9981	2.6 1		24		0.0000E+00
11	2.680		0.0000	0.0000Z	816	282	2.9 1		24		0.0000E+00
12	2.790		0.0000	0.0000Z	23313	10696	2.2 1		24		0.0000E+00
13	2.860		0.0000	0.0000Z	3371	3070	1.1 1		24		0.0000E+00
14	2.950	CB-ACID, ME-ESTER	4206.2461	100.0000Z	2373442	886318	2.7 1	24	24	0	1.7722E-03
15	3.050		0.0000	0.0000Z	74517	38509	1.9 1		24		0.0000E+00
16	3.240		0.0000	0.0000Z	995	296	3.4 1		24		0.0000E+00
17	3.365		0.0000	0.0000Z	9324	3341	2.8 1		24		0.0000E+00
18	3.505		0.0000	0.0000Z	15348	5831	2.6 1		24		0.0000E+00
19	3.595		0.0000	0.0000Z	5397	1869	2.9 1		24		0.0000E+00
20	3.630		0.0000	0.0000Z	1436	852	1.7 1		24		0.0000E+00
21	3.715		0.0000	0.0000Z	5270	1384	3.8 1		24		0.0000E+00
22	3.915		0.0000	0.0000Z	878	396	2.2 1		24		0.0000E+00
23	3.955		0.0000	0.0000Z	8667	2473	3.5 1		24		0.0000E+00
24	4.065	D10-ACID, ME-ESTER	1.9000	0.0000Z	984755	408273	2.4 1	24	24	0	1.0155E-06
25	4.470		0.0000	0.0000Z	58144	12869	4.5 1		24		0.0000E+00
26	4.620		0.0000	0.0000Z	178766	70738	2.5 1		24		0.0000E+00
27	4.745		0.0000	0.0000Z	16227	6998	2.3 1		24		0.0000E+00
28	4.850		0.0000	0.0000Z	37066	11799	3.1 1		24		0.0000E+00
29	4.960		0.0000	0.0000Z	7582	3127	2.4 1		24		0.0000E+00

TOTAL AMOUNT = 4206.2461

AJP000907

EID080329

Start time: 0.00 min. Stop time: 5.00 min. Offset: 0 mv.
 Full Range: 200 millivolts

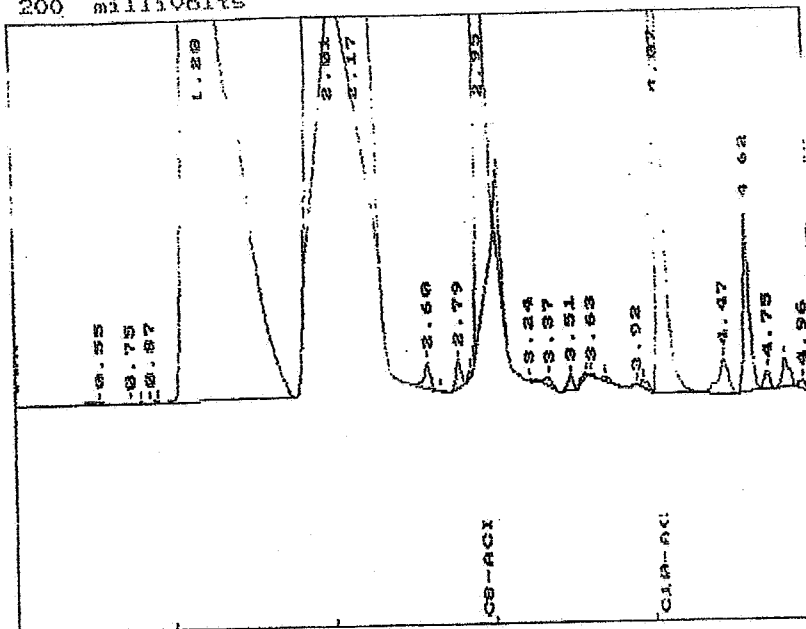

ALP000908

EID080330