

258508 Processed: 03-18-1995 14:18:08, segment 10, cycle 22
 Error, duplicate file name = P:X031722.PTS
 RAW DATA SAVED IN FILE P:X131722.PTS

***** INTERNAL STANDARD TABLE *****
 ***** 03-18-1995 14:18:24 Version 5.1 *****
 * Sample Name: 258508 Data File: P:X131722 *
 * Date: 03-18-1995 14:11:24 Method: M:SEMIDEE 03-18-1995 08:58:58 # 168 *
 * Interface: 4 Cycle#: 22 Operator PD Channel#: 0 Vial#: N.A. *
 * Starting Peak Width: 3 Threshold: 1 Area Threshold: 50 *
 * Instrument Type: HP 5890 2 SEP COLUMN Column Type: DB-5 15M 1.5u film A *
 * Solvent Description: HE DB-1701 30M 0.25ID 0.25u B *
 * Conditions: 60 1MIN-15/MIN FINAL TEMP FID, VARIOUS FOR ECD *
 * Detector 0: FID Detector 1: ECD MU 40 *
 * Misc. Information: INJECTOR A 4psi, B 15 psi *
 Starting Delay: 0.00 Ending retention time: 10.00
 Area reject: 100 One sample per 0.300 sec.
 Amount injected: 1.00 Dilution factor: 1.00
 Internal Standard Amount: 1
 Sample Weight: 1.00000

PEAK NUM	RET TIME	PEAK NAME	CONCENTRATION in PPB	NORMALIZED CONC	AREA	HEIGHT	AREA/ HEIGHT BL	REF PEAK	INT. STD PEAK	% DELTA RET TIME	CONC/AREA
1	0.550		0.0000	0.0000Z	12169	477	25.5 1		27		0.0000E+00
3	0.745		0.0000	0.0000Z	184	179	1.0 1		27		0.0000E+00
4	0.770		0.0000	0.0000Z	612	666	0.9 1		27		0.0000E+00
5	0.825		0.0000	0.0000Z	633	403	1.6 1		27		0.0000E+00
6	0.920		0.0000	0.0000Z	601	379	1.6 1		27		0.0000E+00
7	1.150		0.0000	0.0000Z	4946772	251094	19.7 1		27		0.0000E+00
8	2.075		0.0000	0.0000Z	912811	34865	26.2 1		27		0.0000E+00
9	2.185		0.0000	0.0000Z	304583	43844	6.9 1		27		0.0000E+00
10	2.220		0.0000	0.0000Z	728013	128587	5.7 1		27		0.0000E+00
11	2.470		0.0000	0.0000Z	3326	1723	1.9 1		27		0.0000E+00
12	2.600		0.0000	0.0000Z	23003	9015	2.6 1		27		0.0000E+00
13	2.695		0.0000	0.0000Z	347	184	1.9 1		27		0.0000E+00
14	2.795		0.0000	0.0000Z	107280	48366	2.2 1		27		0.0000E+00
15	2.860		0.0000	0.0000Z	1528	1803	0.8 1		27		0.0000E+00
16	2.960	CB-ACID, NE-ESTER	4222.0293	100.0000Z	2679110	843562	3.2 1	27	27	.2456	1.5759E-03
17	3.050		0.0000	0.0000Z	282188	141901	2.0 1		27		0.0000E+00
18	3.240		0.0000	0.0000Z	856	246	3.5 1		27		0.0000E+00
19	3.320		0.0000	0.0000Z	1583	1041	1.5 1		27		0.0000E+00
20	3.365		0.0000	0.0000Z	3093	1345	2.3 1		27		0.0000E+00
21	3.510		0.0000	0.0000Z	13430	5345	2.5 1		27		0.0000E+00
22	3.600		0.0000	0.0000Z	7078	1468	4.8 1		27		0.0000E+00
23	3.655		0.0000	0.0000Z	1938	1109	1.7 1		27		0.0000E+00
24	3.730		0.0000	0.0000Z	22156	3801	5.8 1		27		0.0000E+00
25	3.820		0.0000	0.0000Z	789	564	1.4 1		27		0.0000E+00
26	3.860		0.0000	0.0000Z	7178	2153	3.3 1		27		0.0000E+00
27	4.070	C10-ACID, NE-ESTER	1107507	0.0000Z	437951	244	1.5 1	27	27		0.0000E+00
28	4.545		0.0000	0.0000Z	325	223	1.5 1		27		0.0000E+00
29	4.405		0.0000	0.0000Z	3812	2212	1.7 1		27		0.0000E+00
30	4.480		0.0000	0.0000Z	29749	9449	3.1 1		27		0.0000E+00
31	4.620		0.0000	0.0000Z	187270	73130	2.6 1		27		0.0000E+00
32	4.750		0.0000	0.0000Z	77711	6531	1.2 1		27		0.0000E+00

AJP000901

EID080323

39 4.763

0.0000

0.00004


5649 2.2 1

21

0.0000E+00

TOTAL ABUNDANT = 4222.0293

Data File = P:\X31722.PTS Printed on 03-18-1995 at 14:18:30
Start time: 0.00 min. Stop time: 5.00 min. Offset:
Full Range: 200 mV/div

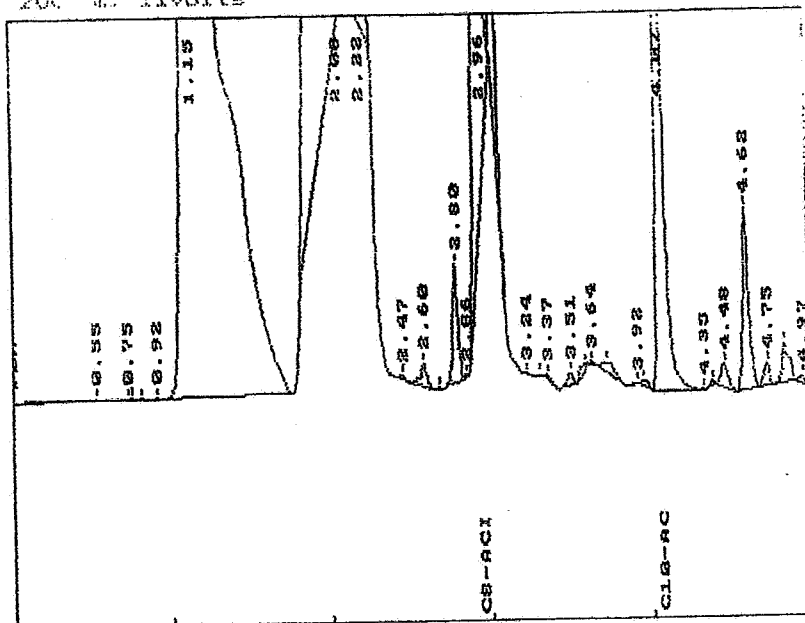

ALP000902

EID080324