

SEMI-VOLATILES ELF Processed: 03-20-1995 18:29:45 Percent 17
 Raw DATA SAVED IN FILE G:F1020101.PTS

***** INTERNAL STANDARD TABLE *****
 ***** 03-20-1995 18:29:57 Version 5.1 *****
 * Sample Name: SEMI-VOLATILES ELF ~~423052~~ Data File: G:F1020101 *
 * Date: 03-20-1995 18:24:43 Method: M:SENIDEE 03-20-1995 12:42:21 # 170 *
 * Interface: 4 Cycle#: 101 Operator PD Channel#: 0 Vial#: N.A. *
 * Starting Peak Width: 3 Threshold: 1 Area Threshold: 50 *
 * Instrument Type: HP 5890 2 SEP COLUMN Column Type: DB-5 15M 1.5u film A *
 * Solvent Description: HE DB-1701 30M 0.25ID 0.25u B *
 * Conditions: 60 1MIN-15/MIN FINAL TEMP FID, VARIOUS FOR ECD *
 * Detector 0: FID Detector 1: ECD MU 40 *
 * Misc. Information: INJECTOR A 4psi, B 15 psi *
 Starting Delay: 0.00 Ending retention time: 10.00
 Area reject: 100 One sample per 0.300 sec.
 Amount injected: 1.00 Dilution factor: 1.00
 Internal Standard Amount: 1
 Sample Weight: 1.00000


PEAK NUM	RET TIME	PEAK NAME	CONCENTRATION in PPB	NORMALIZED CONC	AREA	HEIGHT	AREA/ HEIGHT BL	REF PEAK	INT. STD PEAK	% DELTA RET TIME	CONC/AREA
1	0.555		0.0000	0.0000Z	13520	518	26.1 1		21		0.0000E+00
3	0.845		0.0000	0.0000Z	1048	796	1.3 1		21		0.0000E+00
4	0.935		0.0000	0.0000Z	365	172	2.1 1		21		0.0000E+00
5	1.145		0.0000	0.0000Z	813471	107930	7.5 1		21		0.0000E+00
6	1.285		0.0000	0.0000Z	100448	15045	6.7 1		21		0.0000E+00
7	2.075		0.0000	0.0000Z	998509	21089	47.4 1		21		0.0000E+00
8	2.165		0.0000	0.0000Z	395575	75650	5.2 1		21		0.0000E+00
9	2.245		0.0000	0.0000Z	205939	136197	1.5 1		21		0.0000E+00
10	2.595		0.0000	0.0000Z	29829	11522	2.6 1		21		0.0000E+00
11	2.780		0.0000	0.0000Z	326	287	1.1 1		21		0.0000E+00
12	2.880		0.0000	0.0000Z	864	659	1.3 1		21		0.0000E+00
13	2.945	CB-ACID, HE-ESTER	3987.3413	100.0000Z	2495144	917806	2.7 1	21	21	0	1.5980E-03
14	3.360		0.0000	0.0000Z	8299	2488	3.4 1		21		0.0000E+00
15	3.505		0.0000	0.0000Z	13643	5614	2.4 1		21		0.0000E+00
16	3.570		0.0000	0.0000Z	4121	2319	1.8 1		21		0.0000E+00
17	3.645		0.0000	0.0000Z	1064	597	1.8 1		21		0.0000E+00
18	3.720		0.0000	0.0000Z	11119	2075	5.4 1		21		0.0000E+00
19	3.915		0.0000	0.0000Z	1349	301	4.5 1		21		0.0000E+00
20	3.950		0.0000	0.0000Z	10403	3140	3.3 1		21		0.0000E+00
21	4.060	ClO-ACID, HE-ESTER	1.0000	0.0000Z	1034570	423623	2.4 1	21	21	0	9.6659E-07
22	4.405		0.0000	0.0000Z	4853	2486	2.0 1		21		0.0000E+00
23	4.485		0.0000	0.0000Z	26788	10396	2.6 1		21		0.0000E+00
24	4.615		0.0000	0.0000Z	538393	206412	2.6 1		21		0.0000E+00
25	4.740		0.0000	0.0000Z	2975	1802	1.7 1		21		0.0000E+00
26	4.850		0.0000	0.0000Z	33970	11639	2.9 1		21		0.0000E+00
27	4.960		0.0000	0.0000Z	11928	4592	2.6 1		21		0.0000E+00

TOTAL AMOUNT = 3987.3413

Data File = G:F1020101.PTS Printed on 03-20-1995 at 18:30:02
 Start time: 0.00 min. Stop time: 5.00 min. Offset: 0 mv.
 Full Range: 200 millivolts

EID080352

ALP000915

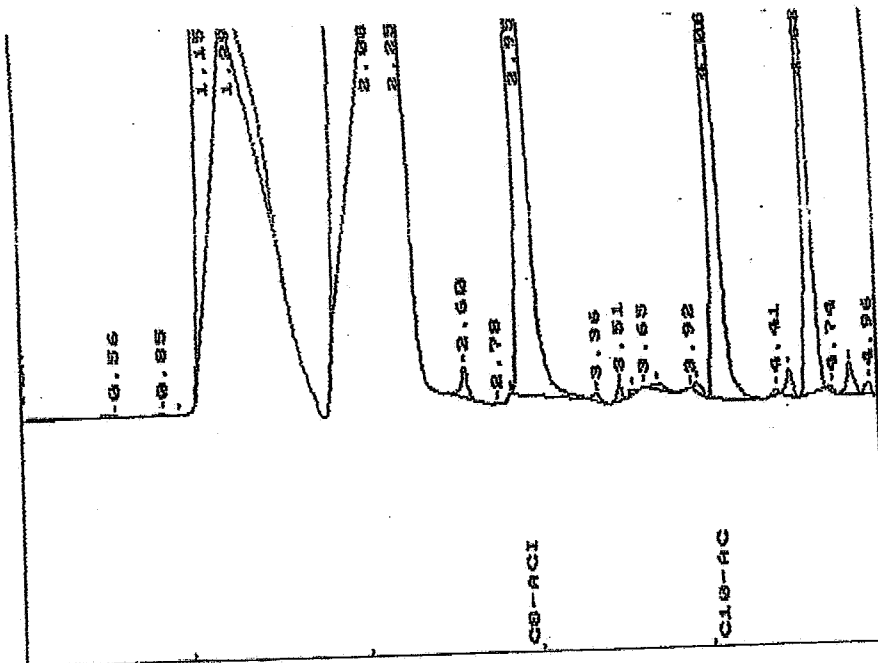

AP000916

EID080353